


# OPERATION MANUAL

## AICHI TURBINE GAS METER

TBX30, TBX100, TBX100F, TBX150F

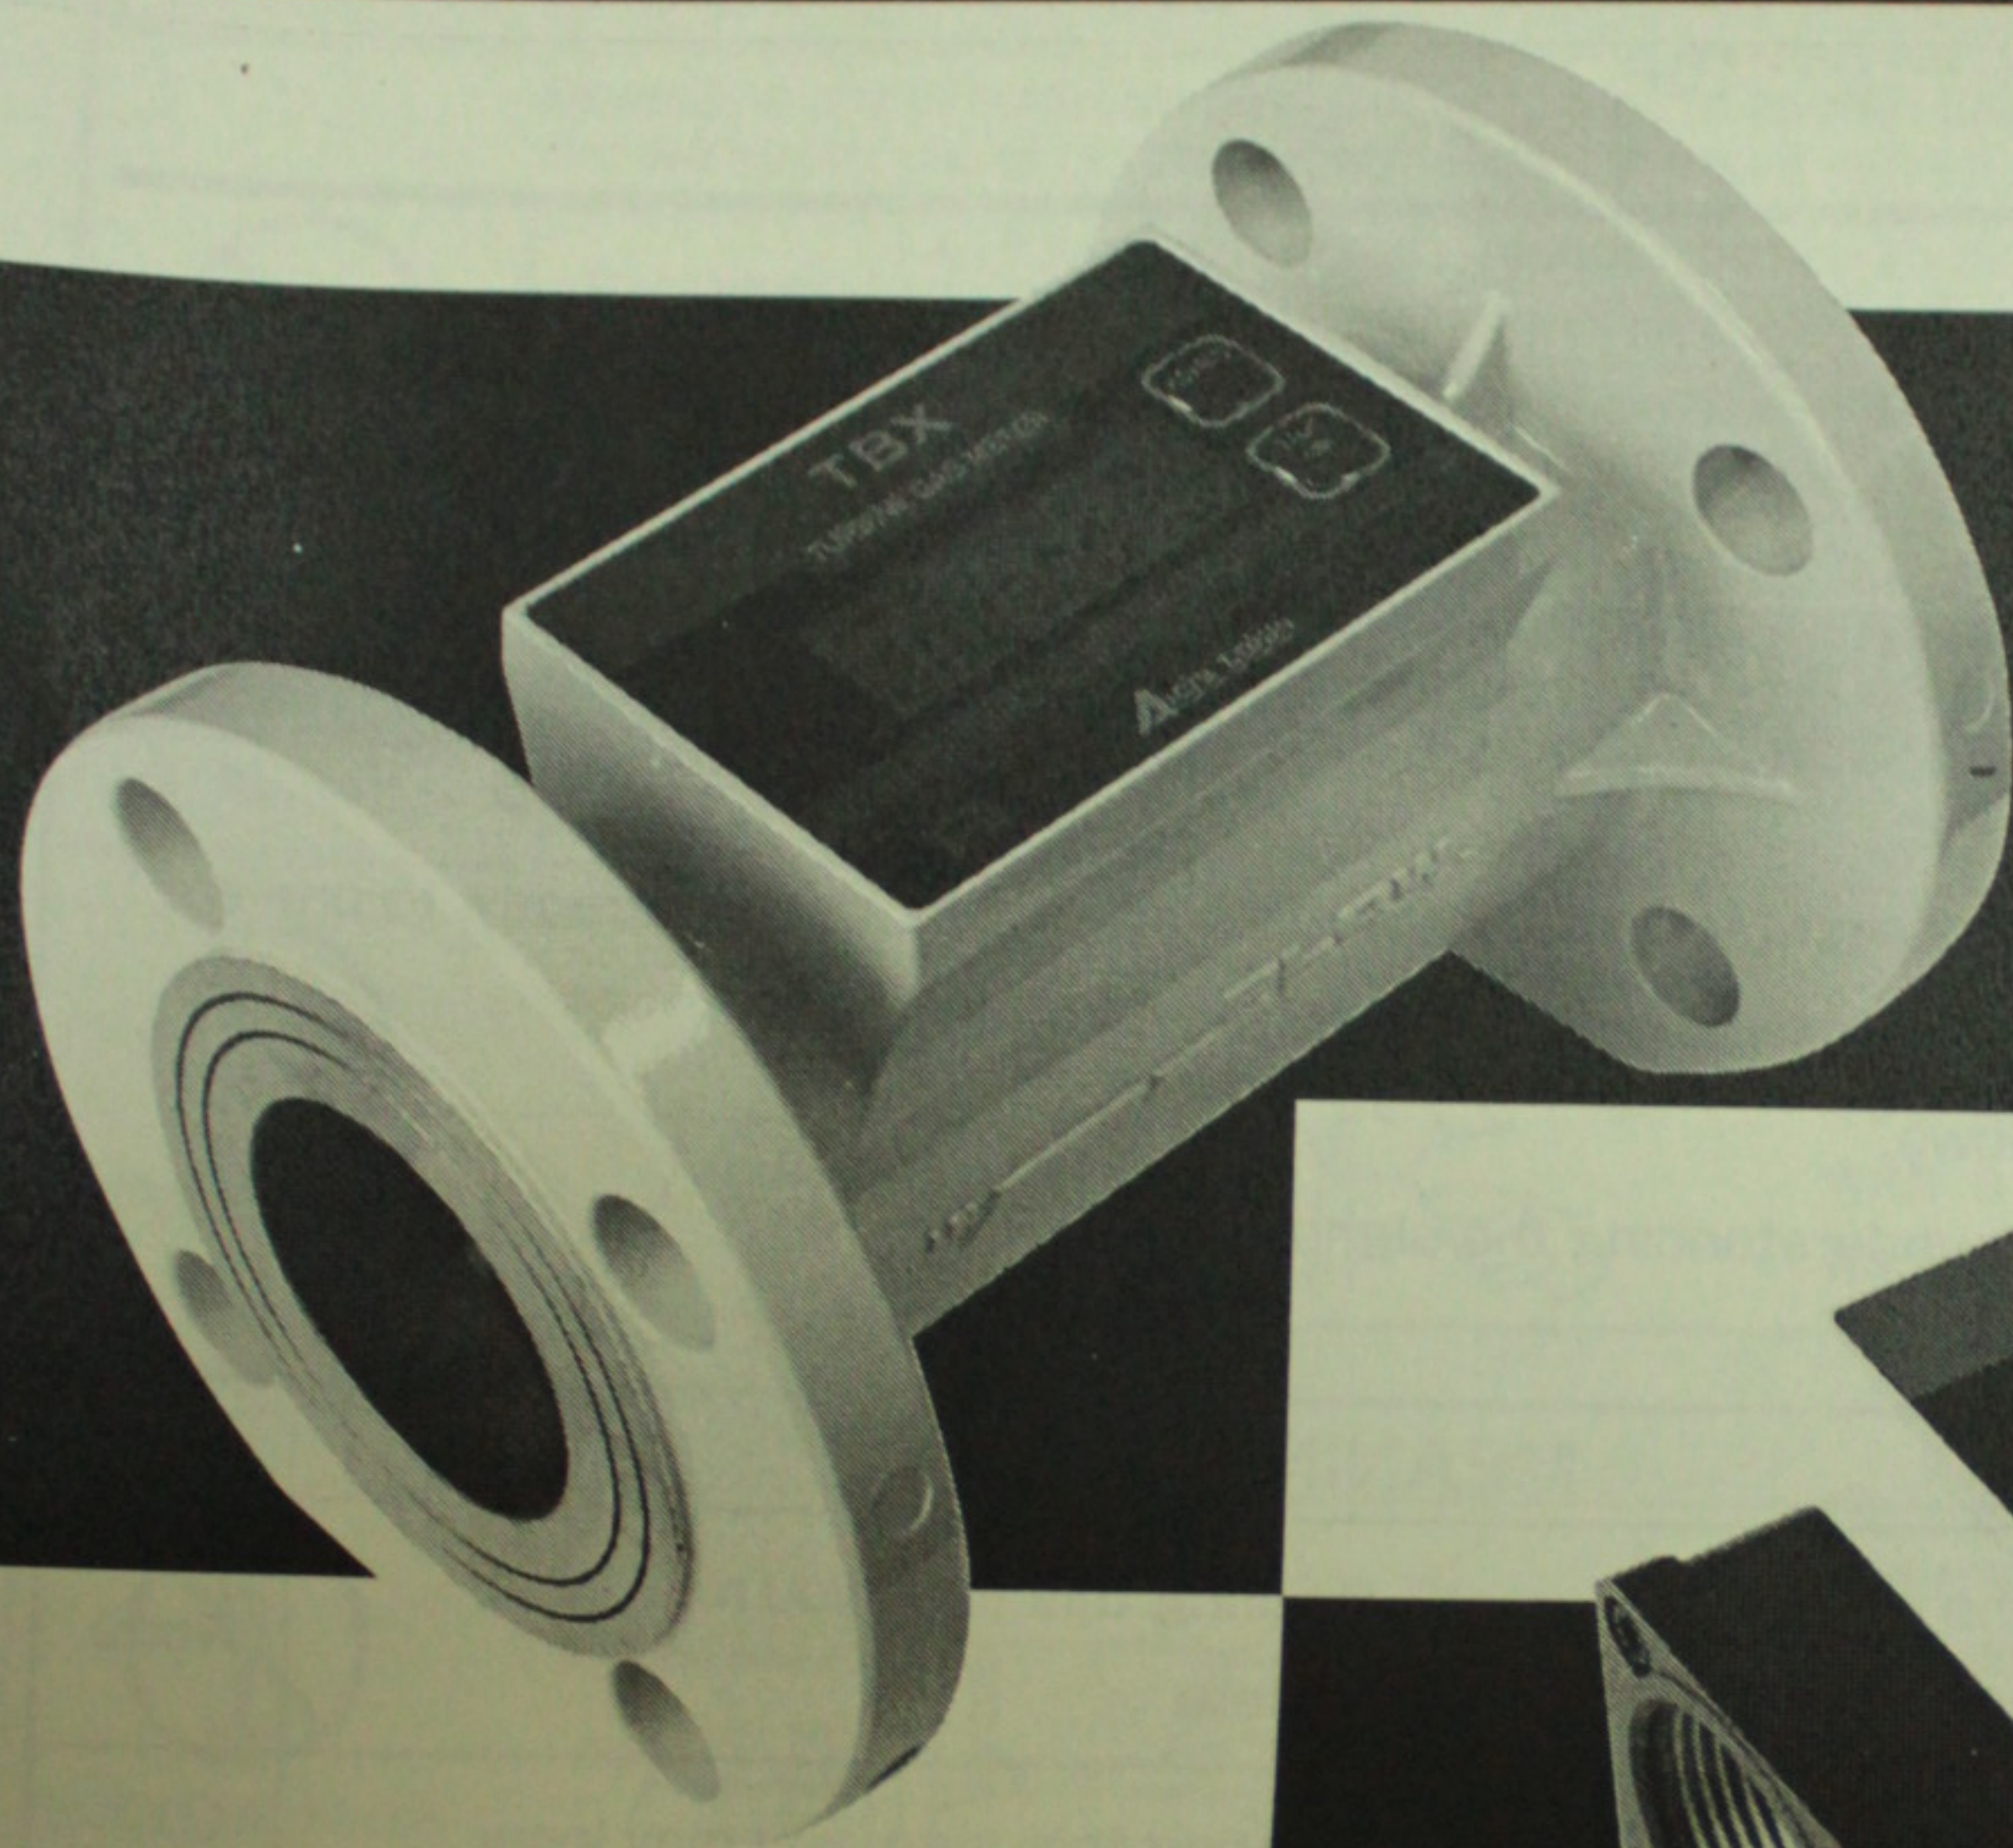

TBX150F




TBX30

Thank you very much for your procurement of  
Aichi Turbine Gas Meter.  
To use the meter correctly, please be sure to read  
this operation manual carefully  
before installation.

# OPERATION MANUAL

## AICHI TURBINE GAS METER

TBX30, TBX100, TBX100F, TBX150F

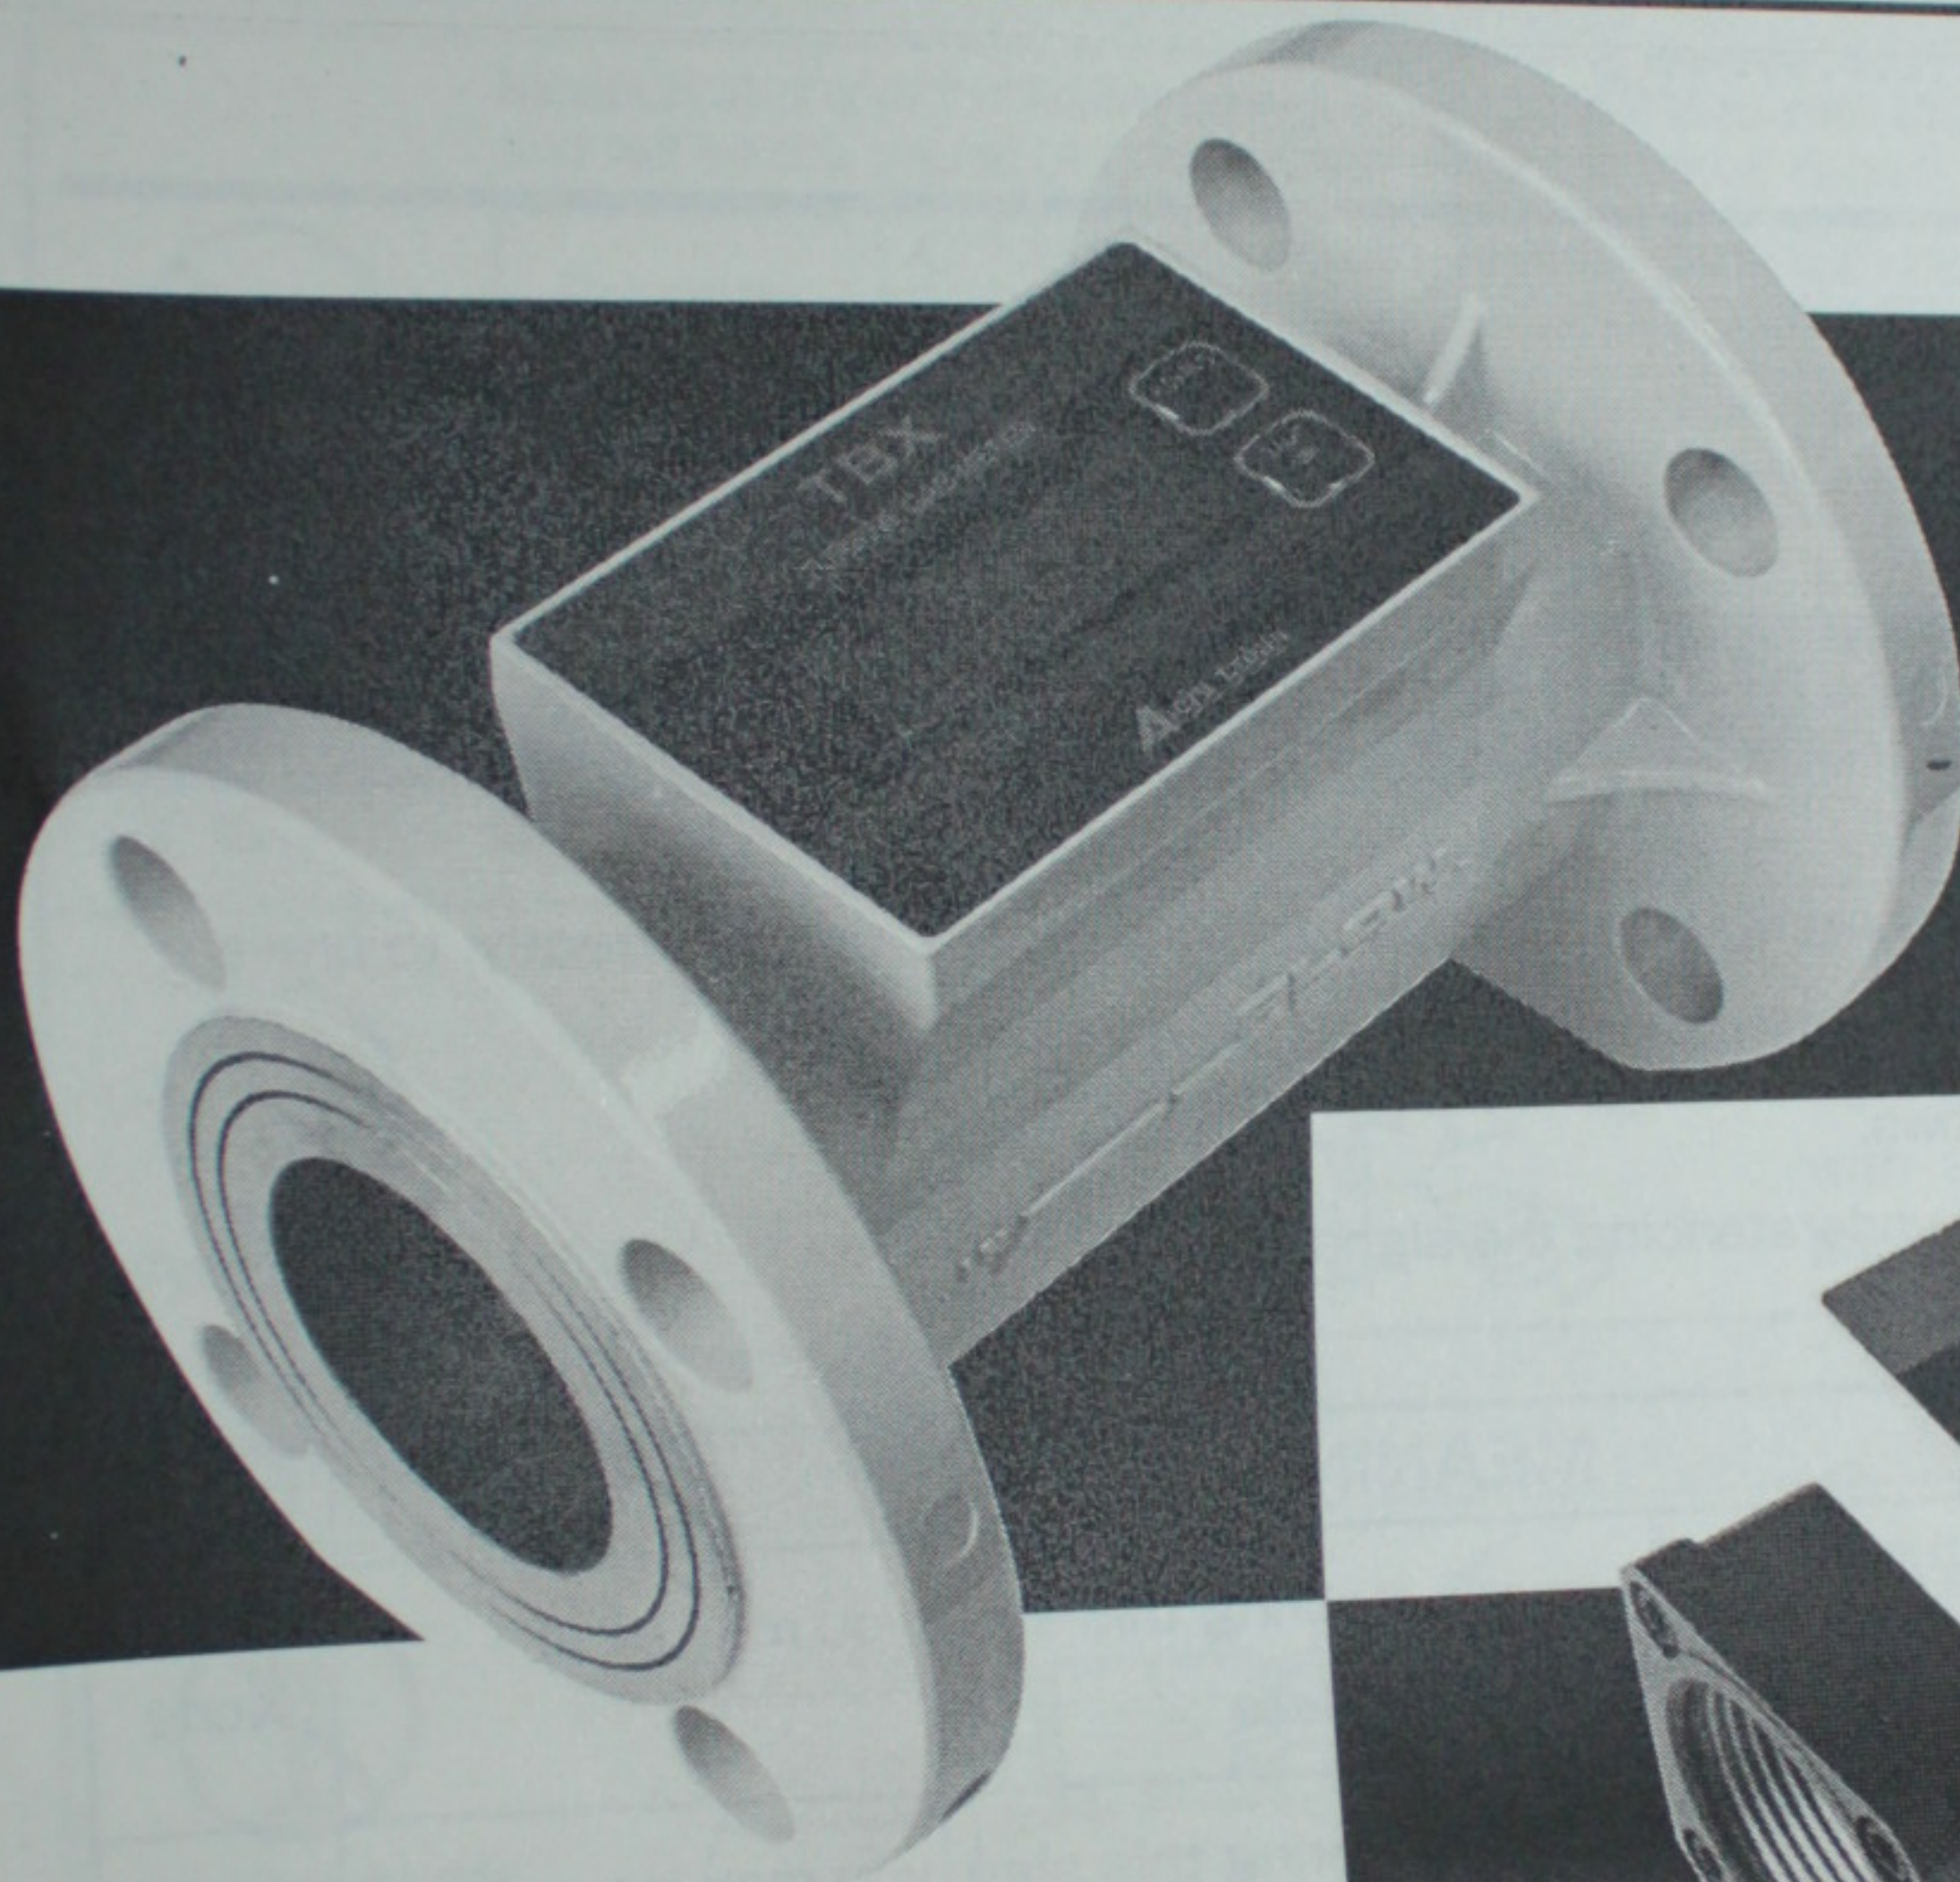

TBX150F



TBX30

Thank you very much for your procurement of  
Aichi Turbine Gas Meter.  
To use the meter correctly, please be sure to read  
this operation manual carefully  
before installation.

**S&S**  
Sensor, System, and Service



**Aichi tokei denki co., ltd.**

# CONTENTS




1. FOR YOUR CORRECT AND SAFE USE .....	1P	9. DIMENSIONS .....	16P
2. SPECIAL CAUTIONS .....	2P	10. SERVICE LIFE .....	16P
3. FOR YOUR CORRECT USE .....	3~4P	11. APPLICATION EXAMPLES .....	17P
4. INSTALLATION AND PIPING PROCEDURE ...	5~6P	12. OUTPUT SIGNAL .....	17P
5. NAMES AND FUNCTION OF DISPLAY ...	7~13P	13. SIGNAL WIRE UNIT (OPTION) .....	18P
6. STARTING OPERATION PROCEDURE .....	14P	14. REMOTE DISPLAY / COUNTER (OPTION) ...	19P
7. INSPECTION PROCEDURE .....	14P	15. WARRANTY .....	20P
8. SPECIFICATIONS .....	15P		

## 1. FOR YOUR CORRECT AND SAFE USE

This operation manual uses various picture signs for you to use the Turbine Gas Meter correctly, to prevent injuries on yourself and other people, and also to prevent damage to properties.

The signs and their meanings are as follows.

Please proceed to instructions after fully understanding the signs.

SIGN	MEANING	PAGE
 DANGER	If you operate the product incorrectly ignoring this sign, you may incur imminent danger of death or serious injuries.	None
 WARNING	If you operate the product incorrectly ignoring this sign, you may incur danger of death or serious injuries.	None
 CAUTION	If you operate the product incorrectly ignoring this sign, you may incur injuries or material damage.	2


Each picture sign has the following meaning



Caution  
In  
General



Do Not  
Touch

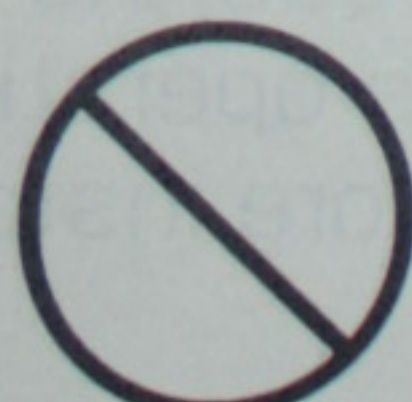

Prohibition  
In General



Do Not  
Disassemble



No Fire



Do  
Without  
Fail

Page

2·4·9·14·16

—


2·4

2

—


2·3·4·9

## 2. SPECIAL CAUTIONS

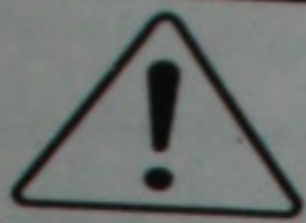

### CAUTION


#### 1. Do not install the meter in any dangerous place

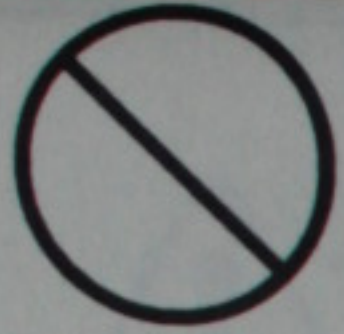

Prohibition

The electric circuit of the meter is not explosion proof structure.

#### 2. Do not use the meter for measuring any of corrosive gases or following gases

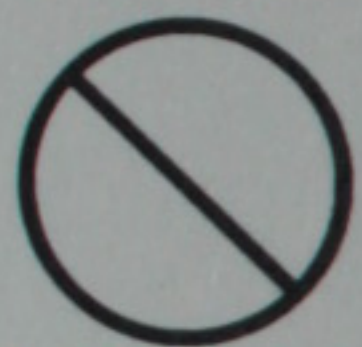


Prohibition

Measuring any of corrosive gases or following gases with the meter will cause corrosion of its parts and will be the cause of gas leakage. Also, the meter cannot measure these gases correctly.


Poisonous gas	Chlorine, Hydrogen cyanide, Nitrogen dioxide, Fluorine
	Hydrogen chloride, Boron trifluoride, Boron dioxide
	Sulfur dioxide, Hydrogen fluoride, Sulfur sulfide
Others	Ammonia, Chlorine dioxide, Oxygen, Hydrogen, Helium

Deterioration of the meter performance or damage on the meter may be caused by measuring gases having certain physical prosperities. Please check us in case of measuring special gas.

#### 3. Do not give the meter a shock

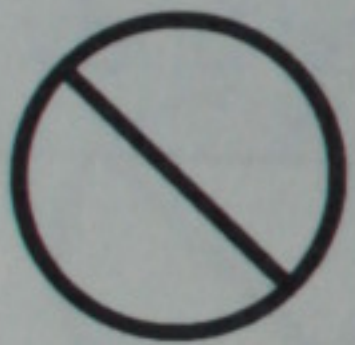

Prohibition

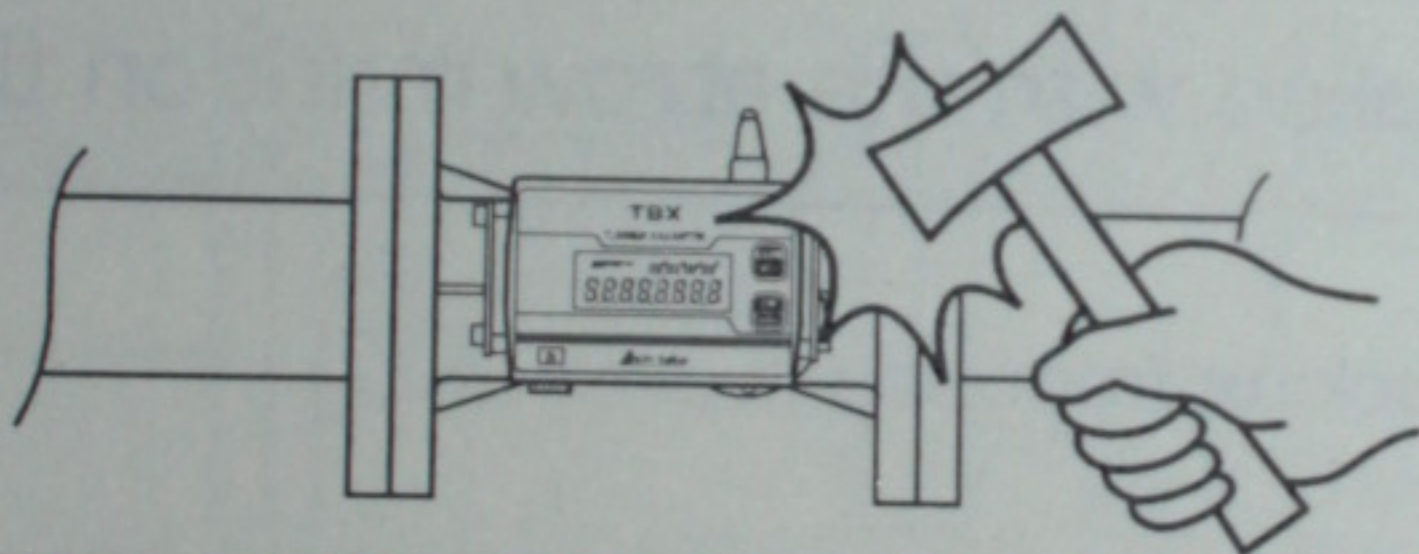


The meter is a precision measuring instrument. Do not give the meter a strong shock. Also, do not hit the meter with a thing. They will be the cause of gas leakage and/or damage.

#### 4. Do not disassemble the meter



Do Not Disassemble

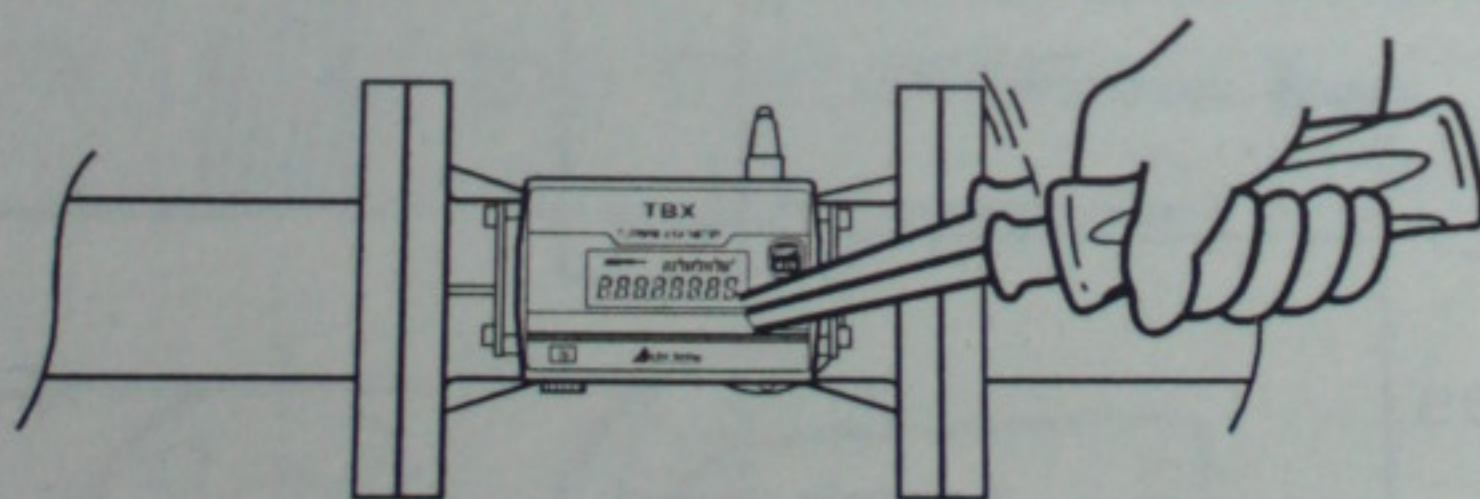


The meter is a precision measuring instrument.  
Do not disassemble the meter.  
It will be the cause of gas leakage.

#### 5. After installation of the meter, execute an airtight test of the portion including pipes, etc., in the upstream and the downstream of the meter



Do Without Fail

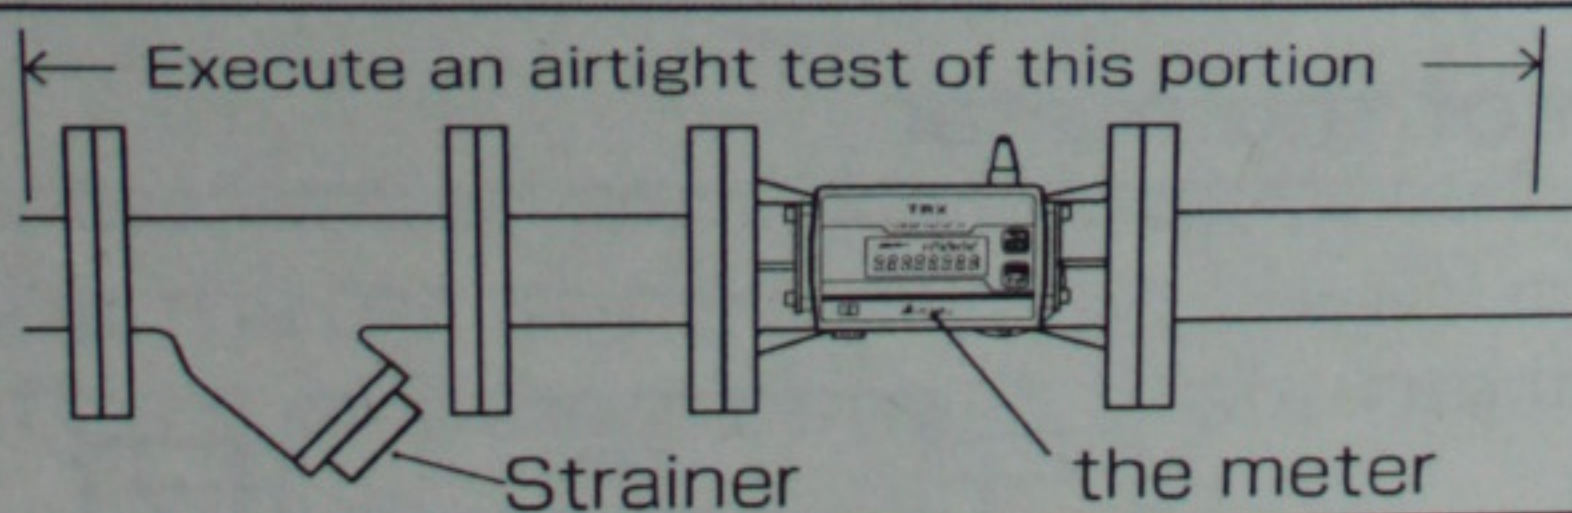

Please check there is no leakage at pressure of  $1.1 \times$  Maximum Working Pressure.

#### 6. Disposal of the used meter




Do Without Fail

For our collection of the waste lithium battery, please send the meter back to us after finishing its use.  
Or, please disposal the lithium battery as industrial waste after complete discharge of its electricity.

# 3. FOR YOUR CORRECT USE

1. Check the specifications on the name plate are suitable to your working conditions

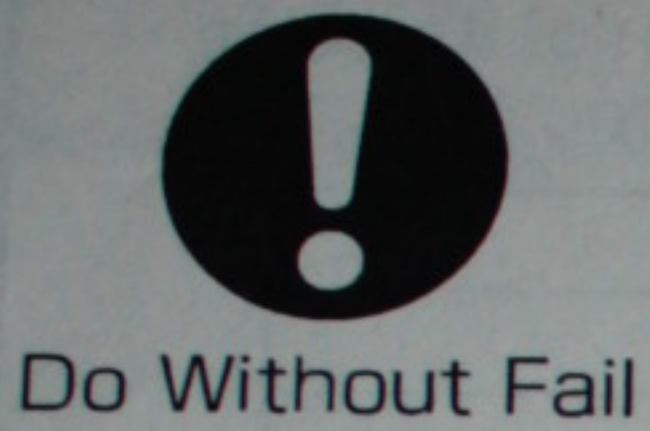

Do Without Fail

Model	TBX150 F-L
Range	12.5~150 m <sup>3</sup> /h
Max. Pressure	100 kPa
Temperature	-10~60°C
Standard point	actual
Output A[B]	0.10 m <sup>3</sup> /P [461.6 $\frac{cm^3}{p}$ ]
Pulse width A	40ms
Date	'06-09
Serial No.	0002397

**Aichi tokei denki co., ltd.**


- Model
- Flow range
- Maximum working pressure
- Working temperature range
- actual
- Unit pulse
- High-density pulse
- Output pulse width
- Year and month manufactured
- Serial number

2. Make the gas flow direction be complied with the arrow mark on the meter body

Drawing looking from side




Do Without Fail

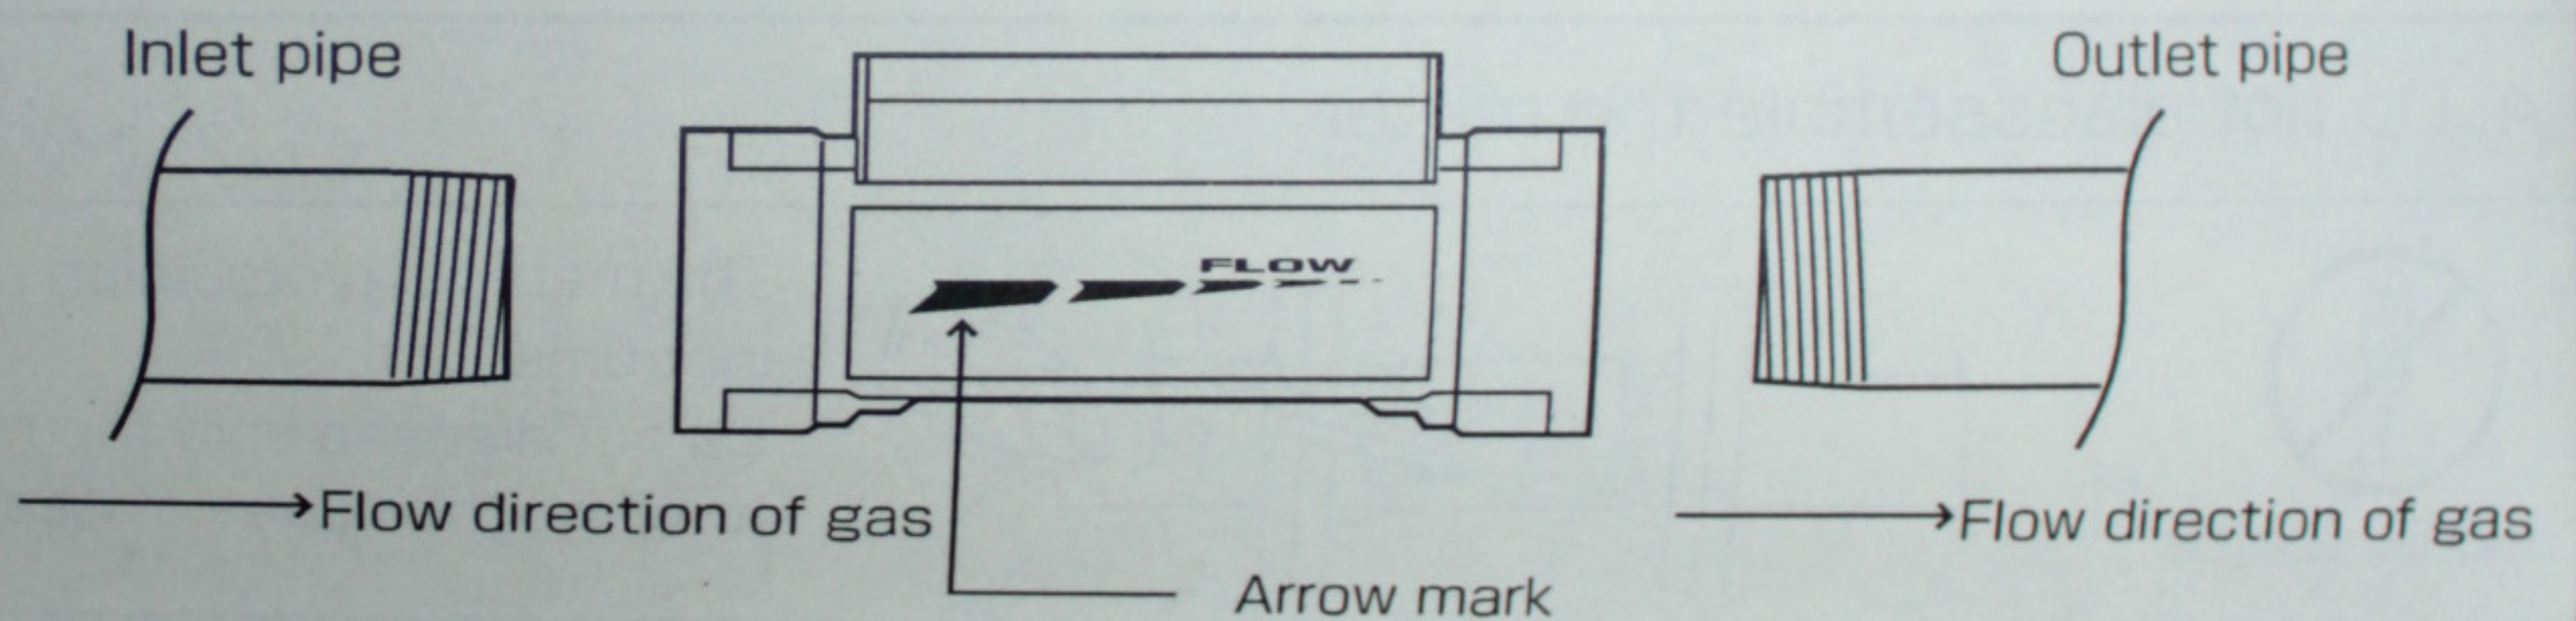

3. Install a strainer at the upstream of the meter




Do Without Fail

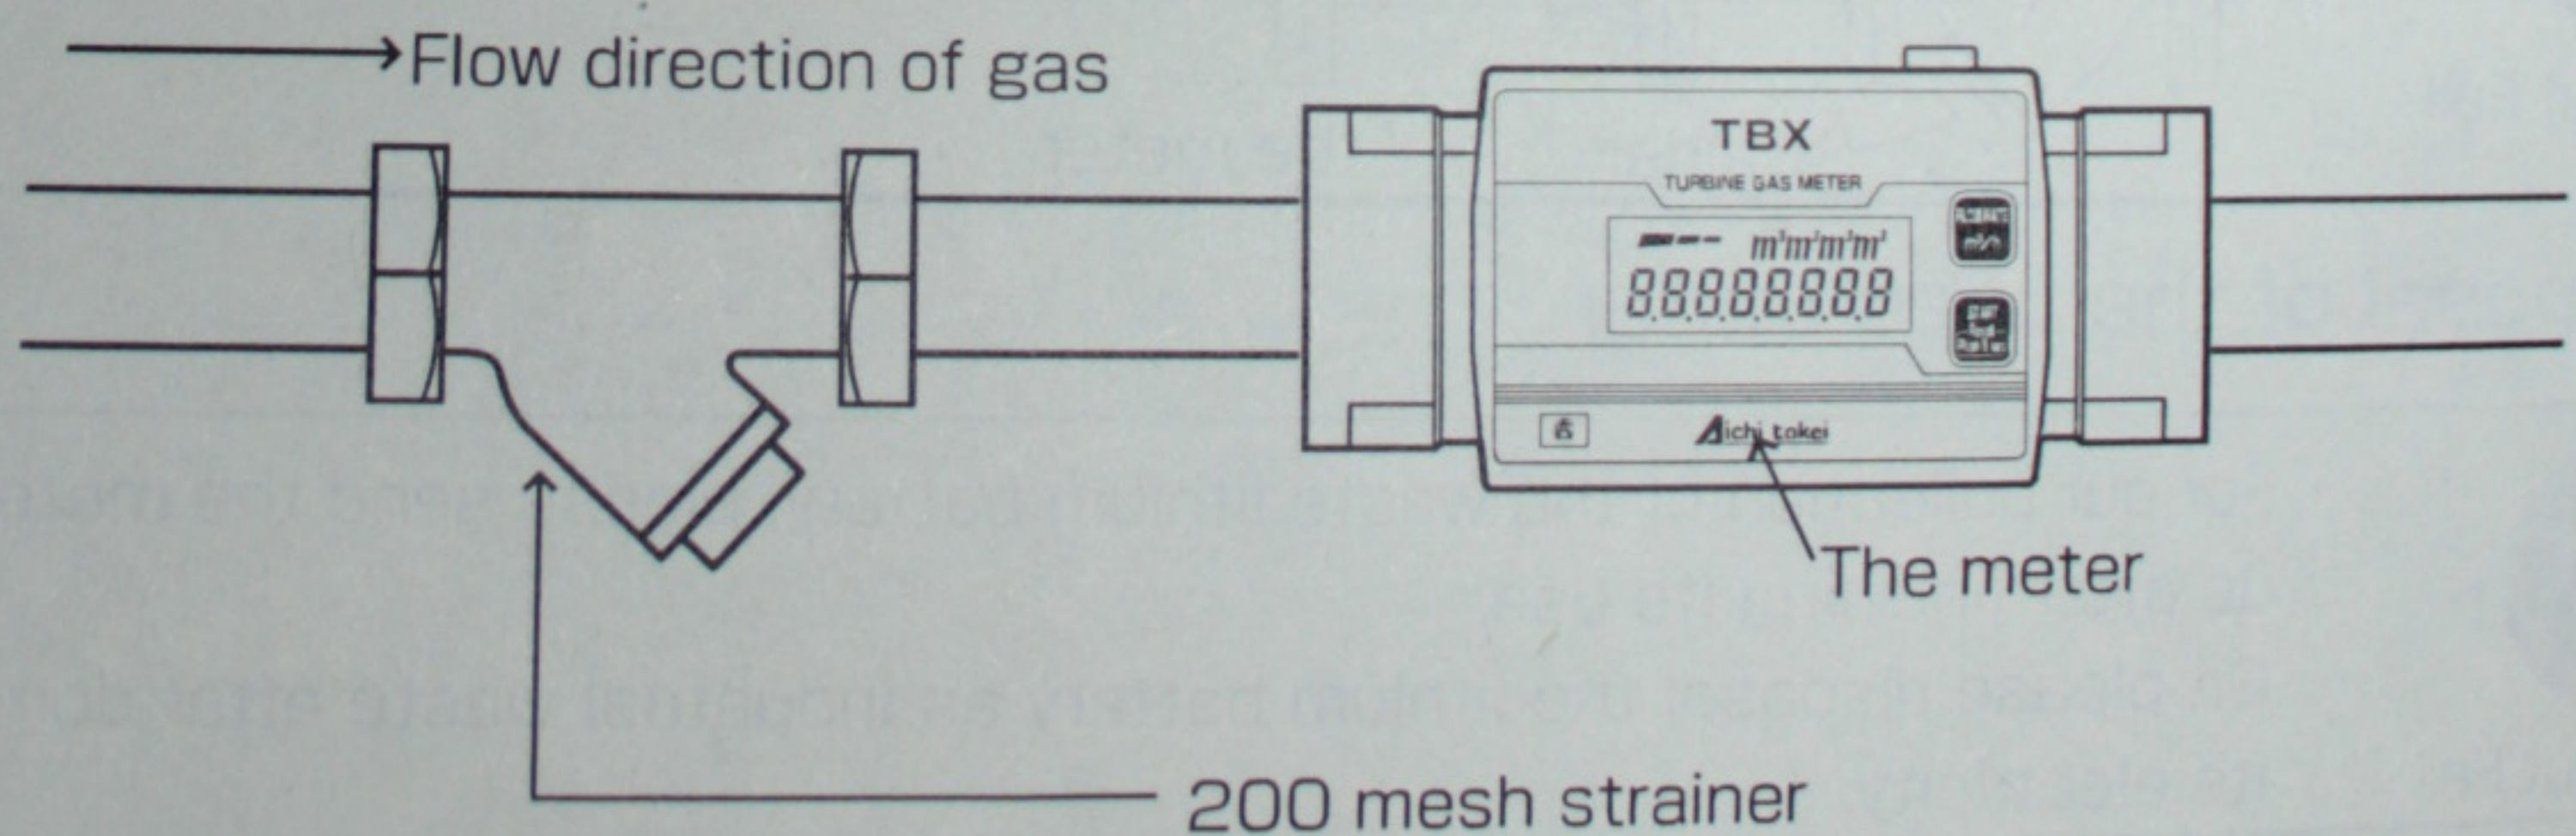


#### 4. Do not install the meter in a place where oil mist and/or dust powder, etc., waft


- ① Using the meter with LP Gas (Liquid Petroleum Gas) produced by a vaporizer may cause abnormality of the meter's turning parts because of oil mist (adhesive substance due to re-liquefaction) in pipes. And as the result, the meter may be impossible to measure correctly.

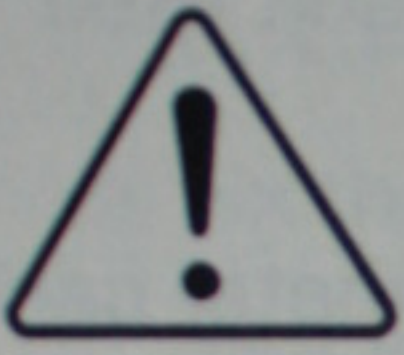


Caution

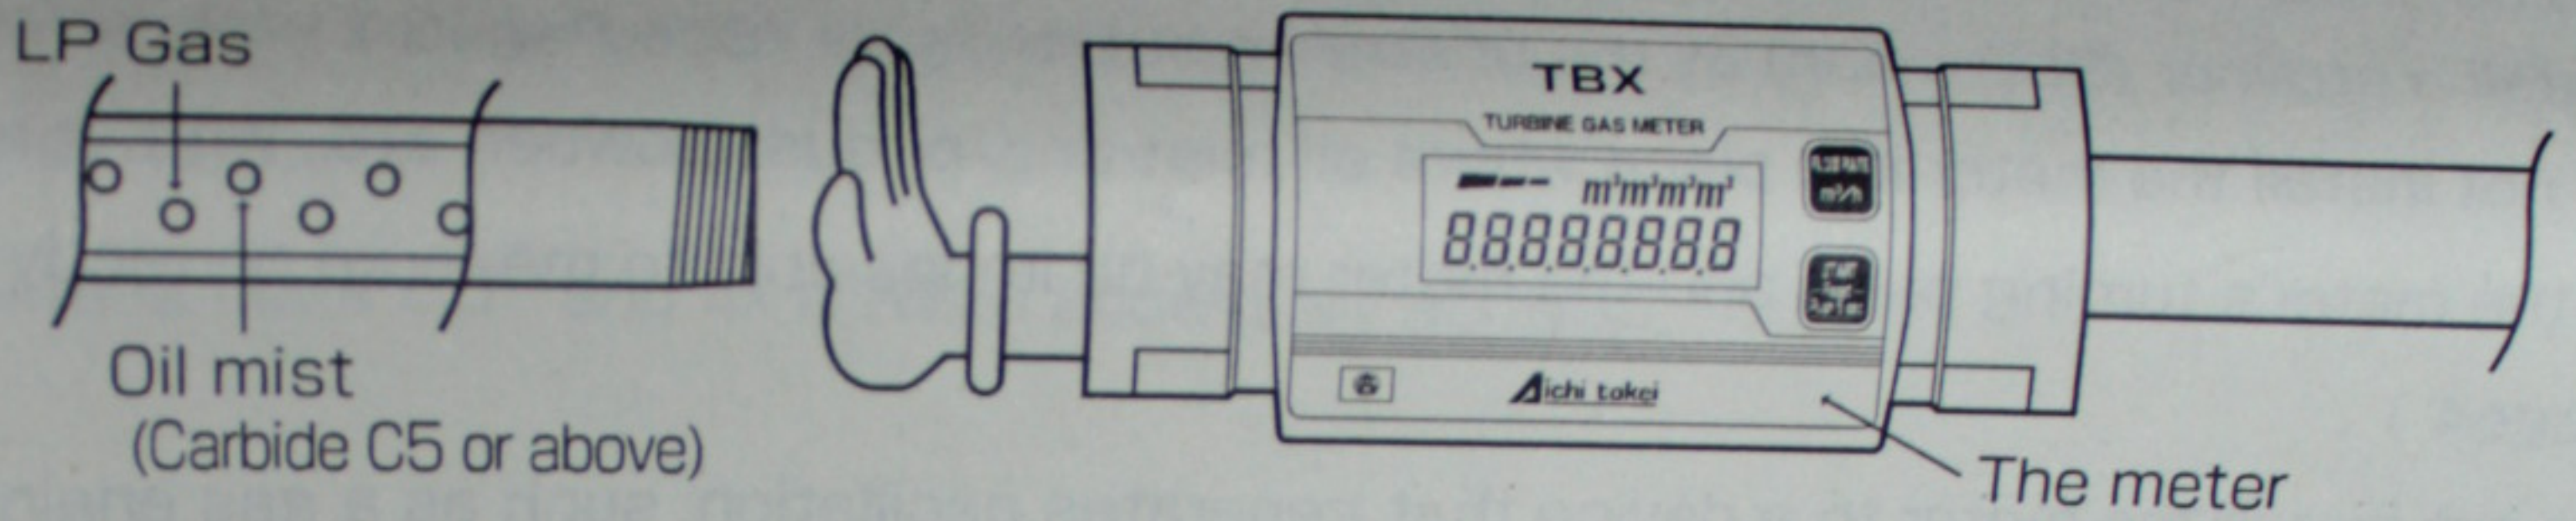


- ② Using the meter for dry gas (13A Gas, etc.) may cause abnormality of the meter's turning parts because of dust powder (Powdery foreign substance) in pipes. And as the result, the meter may be impossible to measure correctly.

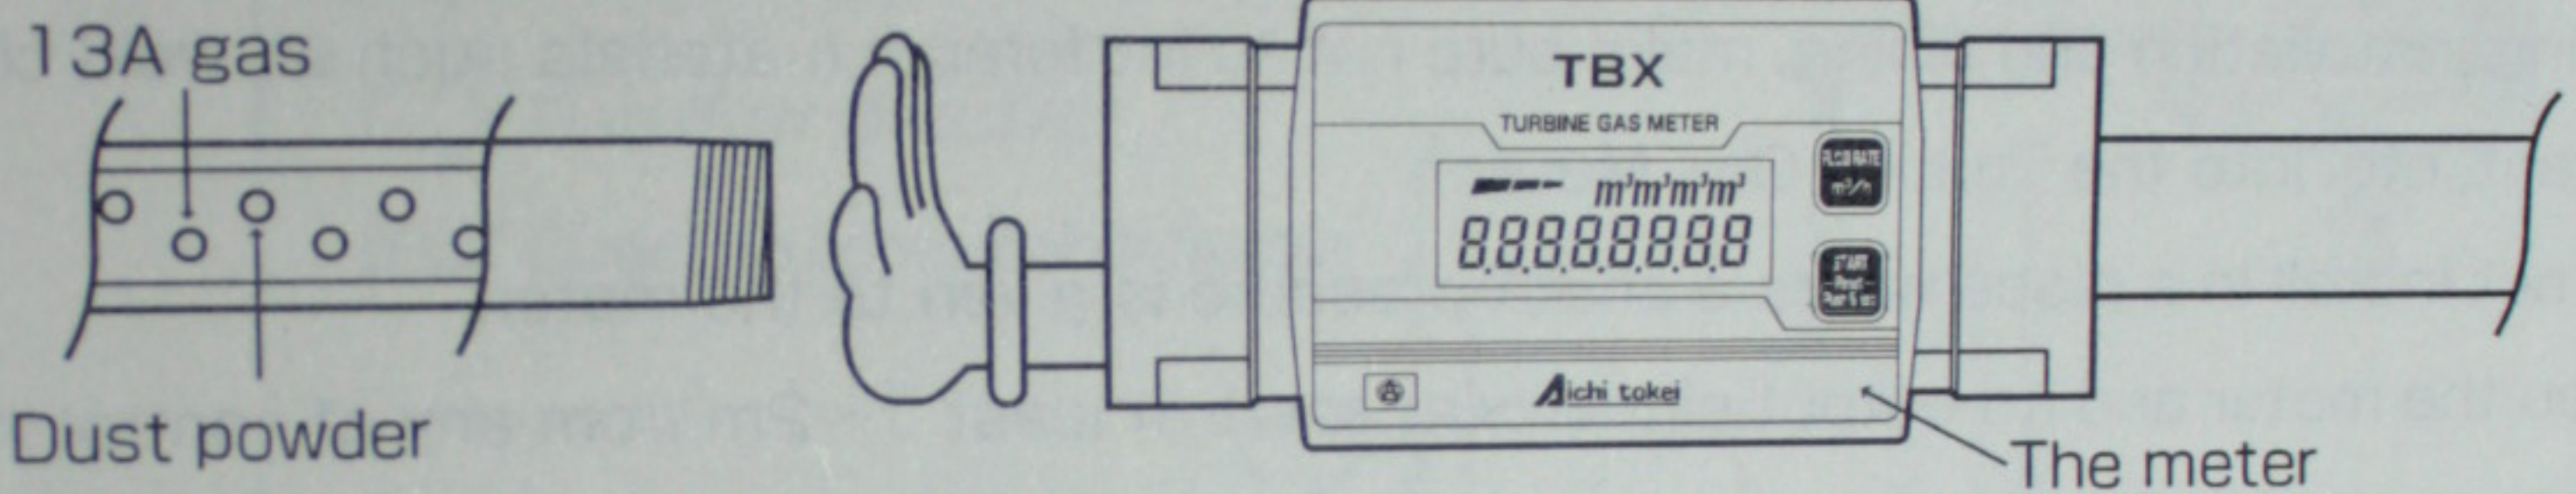

#### 5. Do not tighten the flange nuts excessively at the time of the meter installation

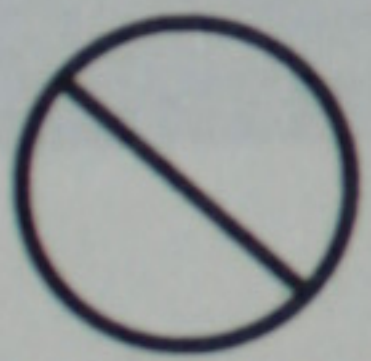

Prohibition

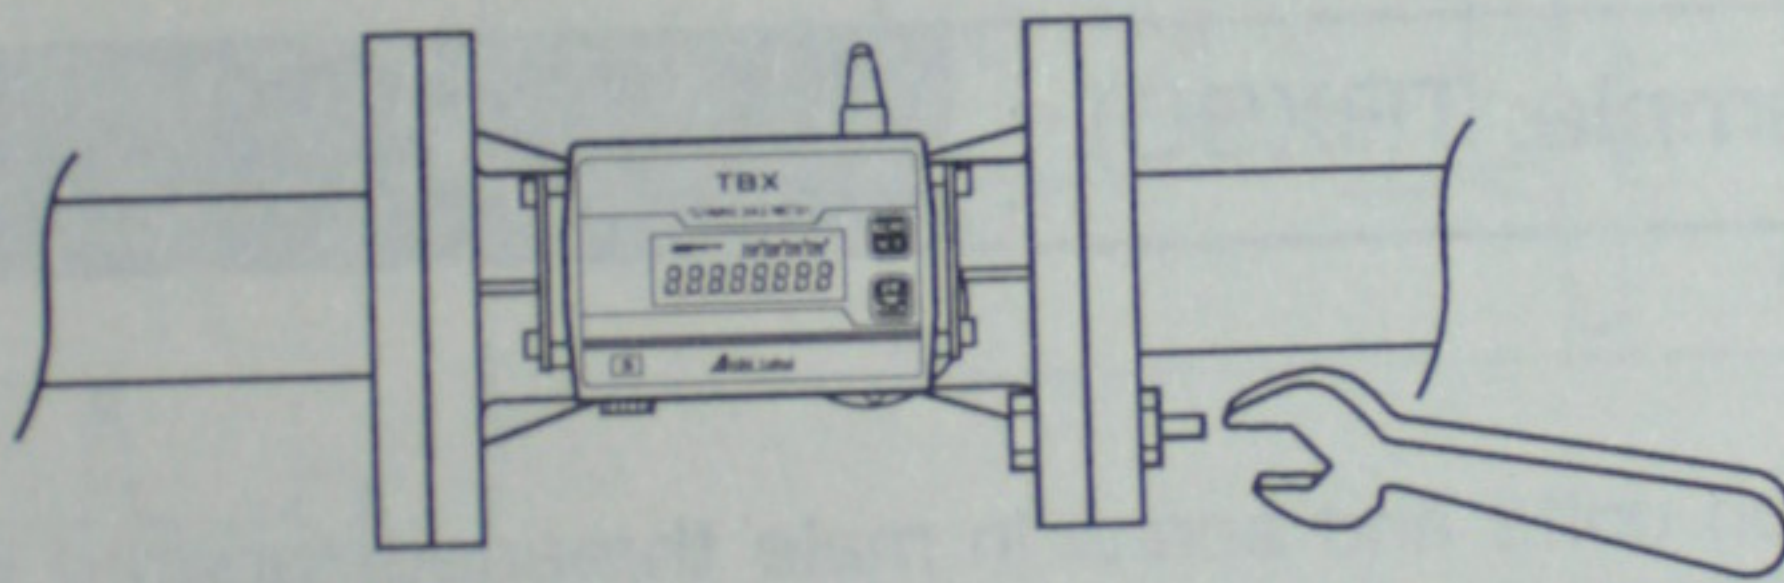


After lightly tightening all the nuts, tighten them diagonally with equal power. (For TBX100F and TBX150F)

#### 6. To connect the meter flanges to companion flanges, adjust the center of the meter body to the same of companion pipes



Do Without Fail


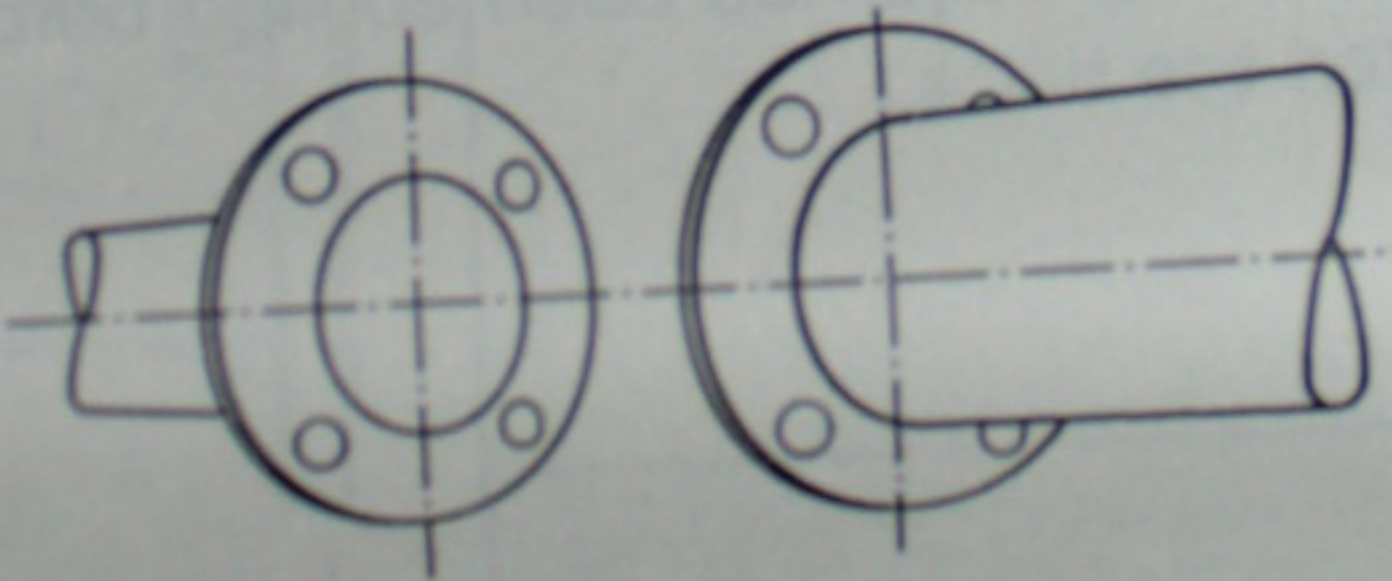


Avoid eccentricity of the center of the meter body from the same of companion pipes. And, avoid inclining and distortion of the flanges. Also, do not give excessive stress load to the meter body. (For TBX100F and TBX150F)

#### 7. To install the meter in new piping, execute dust purge to remove foreign matters in pipes before the installation



Do Without Fail

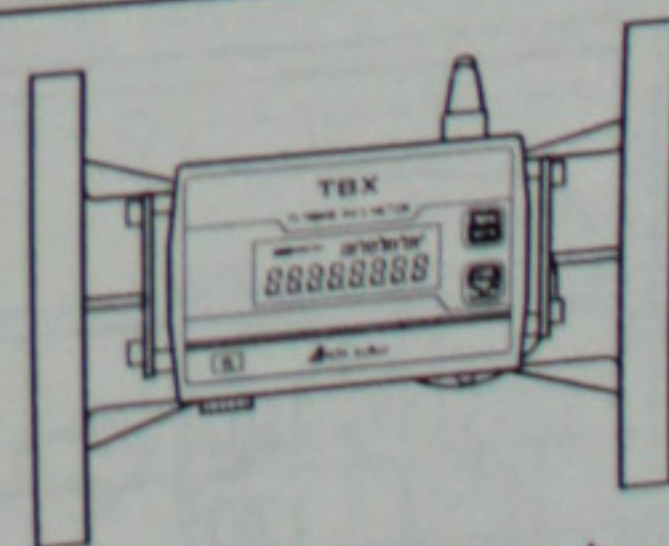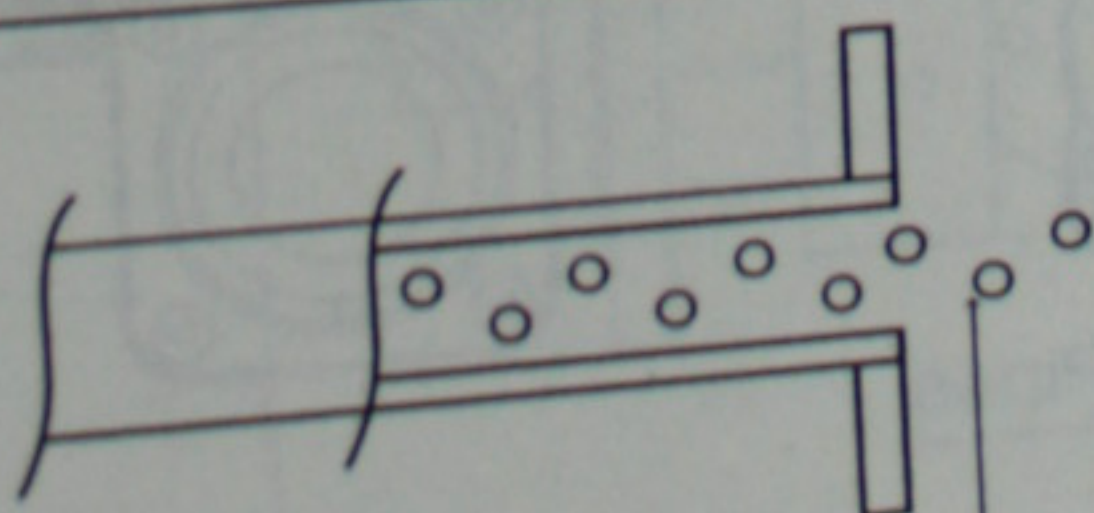

Remove welding chips and dust

## 4. INSTALLATION AND PIPING PROCEDURE

1. The Turbine Gas Meter is of indoor type. Install it in a place not exposed to rainwater.
2. The meter can be installed both horizontally and vertically. Install it in between straight pipes.
3. Do not install the meter in a place where there is possibility of remaining of liquid such as oil, water, etc.
4. Install a strainer (200 mesh) at the upstream of the meter (See Page3 ).
5. Do not install the meter in a place where oil mist and/or dust powder, etc., waft. It may cause abnormality of the meter's turning parts and the meter may be impossible to measure correctly as the result (See Page4 ) .
6. Do not install the meter to a device that generates oscillation, such as a gas engine, as the meter cannot measure correctly.
7. Provide at least 10D (10×Meter's Nominal Diameter) straight pipes at the upstream and the downstream of the meter.
8. During installation and piping, make sure not to let foreign materials such as weld chips, dirt, waste sealant, etc. into the Turbine Gas Meter.
9. Do not install in a place where a shock pressure is given to the meter.
10. Keep the meter and its output signal wire apart at least 1~2m from any of control instruments (ex: an electromagnetic valve), noise sources (ex: a power cable), etc.
11. Direction of the display can be selected according to your piping.


### ① Thread Connection Type (Example: TBX30)

#### (1) Installation

To install the meter, fix the connection units and screw in male threaded tapered pipes to the both sides of the meter.

#### (2) Maintenance

- ① By detaching the bolts (8 bolts) at the outer side of the connection units, the meter body can be drawn out in the direction perpendicular to the pipes.
- ② After replacing the O-rings with new ones to which grease has been applied beforehand, install the meter body to the connection units. And, tighten the bolts.

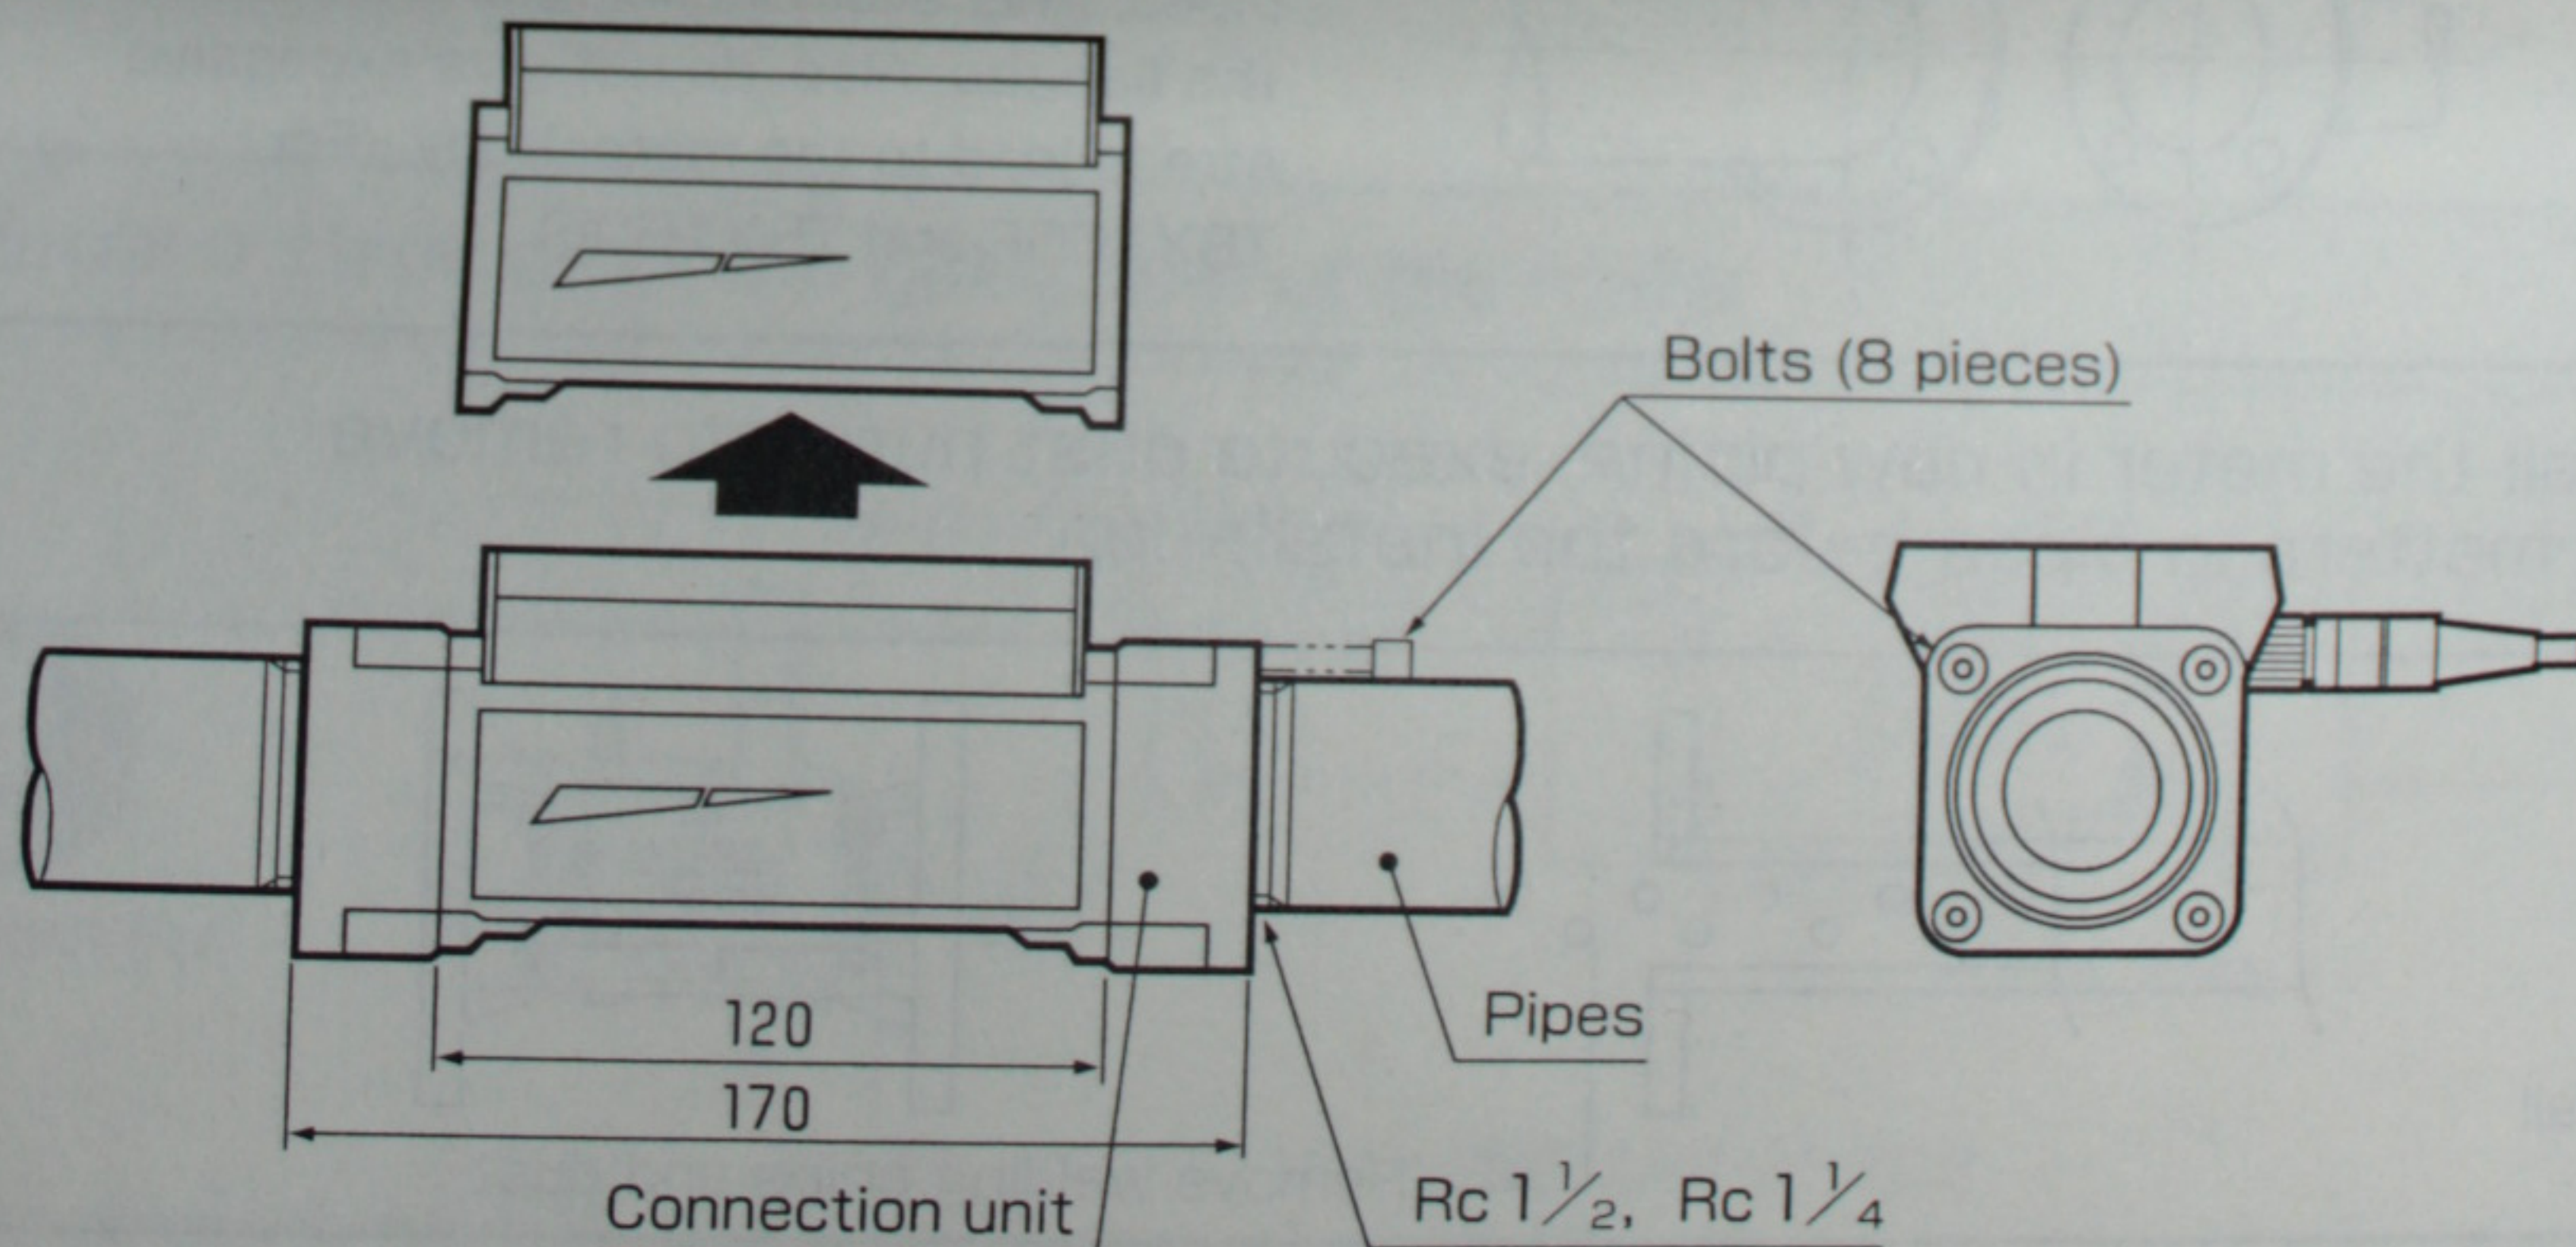


## Flange Connection Type (Example: TBX100F)

The display of the Turbine Gas Meter can be turned round so as to match it to the direction of a gas flow. Also, the display can be removed from the meter body to use it as the remote display. To turn round the display,

- ① Remove the hexagonal socket bolts on the both sides of display.
- ② A. Fix the mounting plate on the wall (With accessory screws).  
B. Turn the display 180°.  
C. Turn the mounting plate 90° and fix it (With accessory screws).
- ③ Fix the counter.

The display can be placed at an angle of maximum 10° (approx.).

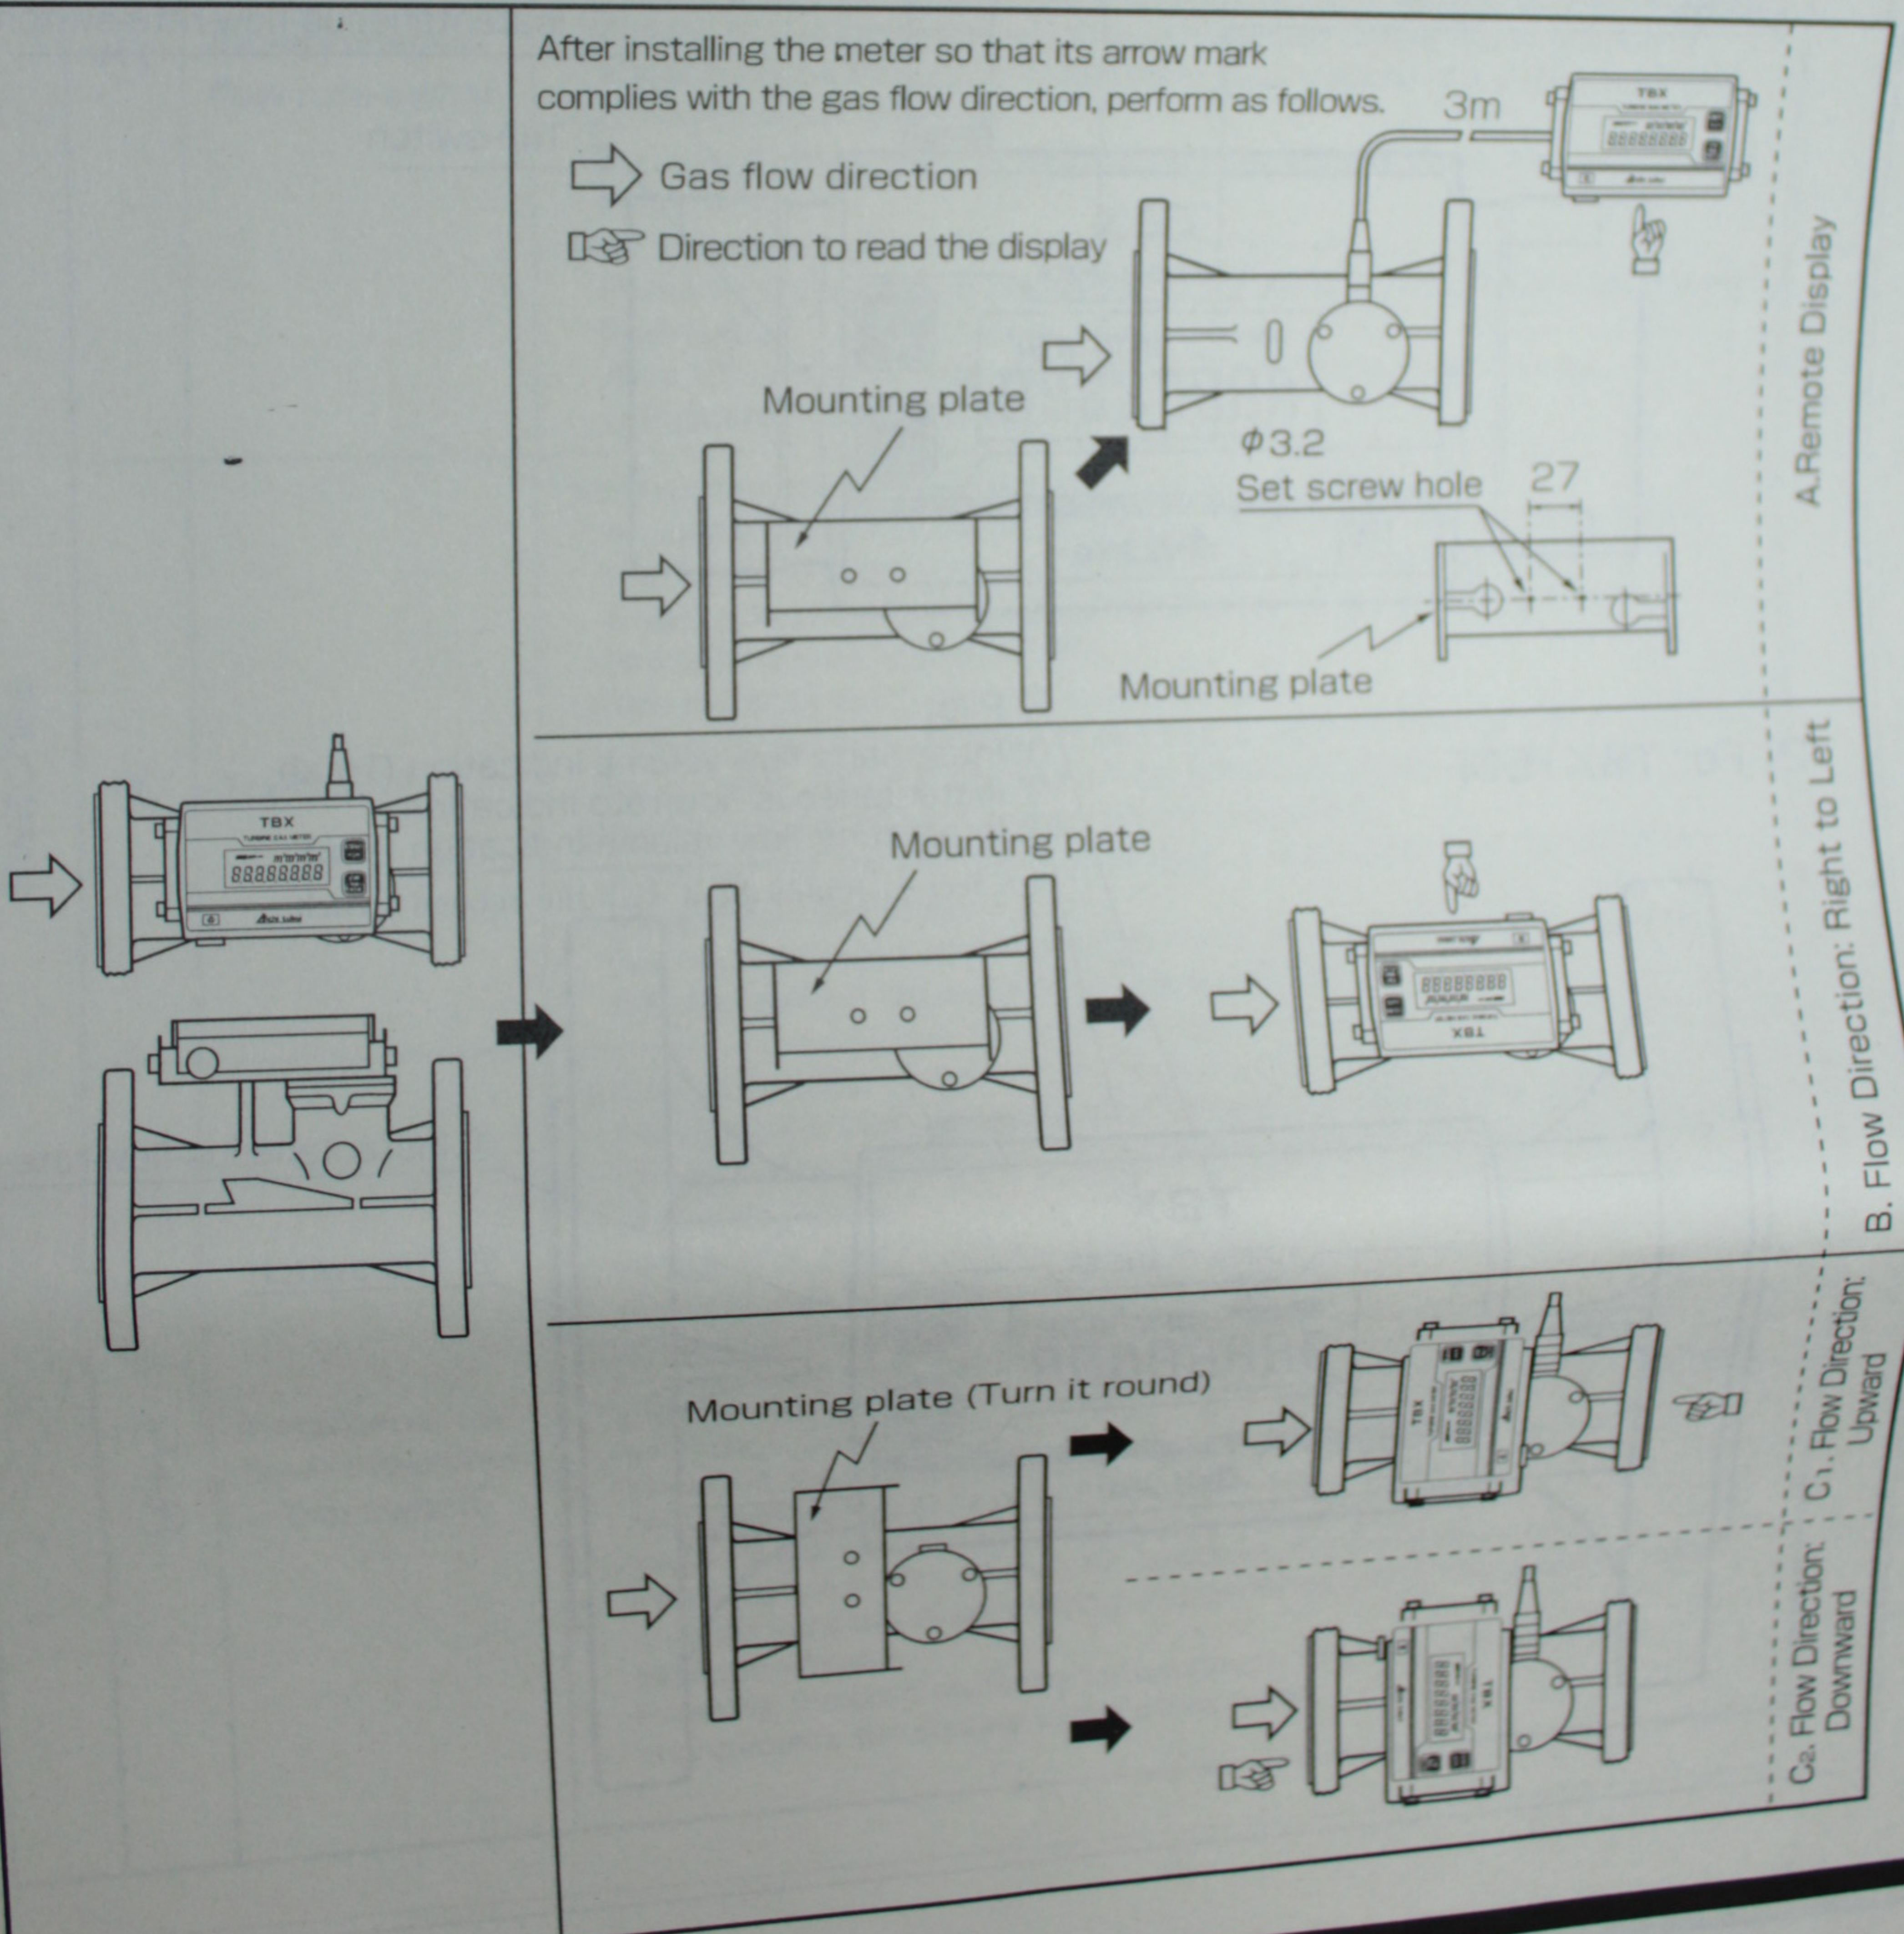




# 5. NAMES AND FUNCTION OF DISPLAY


## 1) For TBX30, TBX100, and TBX100F

- ③ Integrating flow volume indication (Total)
- ④ Instantaneous flow-rate indication
- ⑤ Integrating flow volume indication (Trip)
- \* Select each indication with the related switch.
- ⑥ Pilot

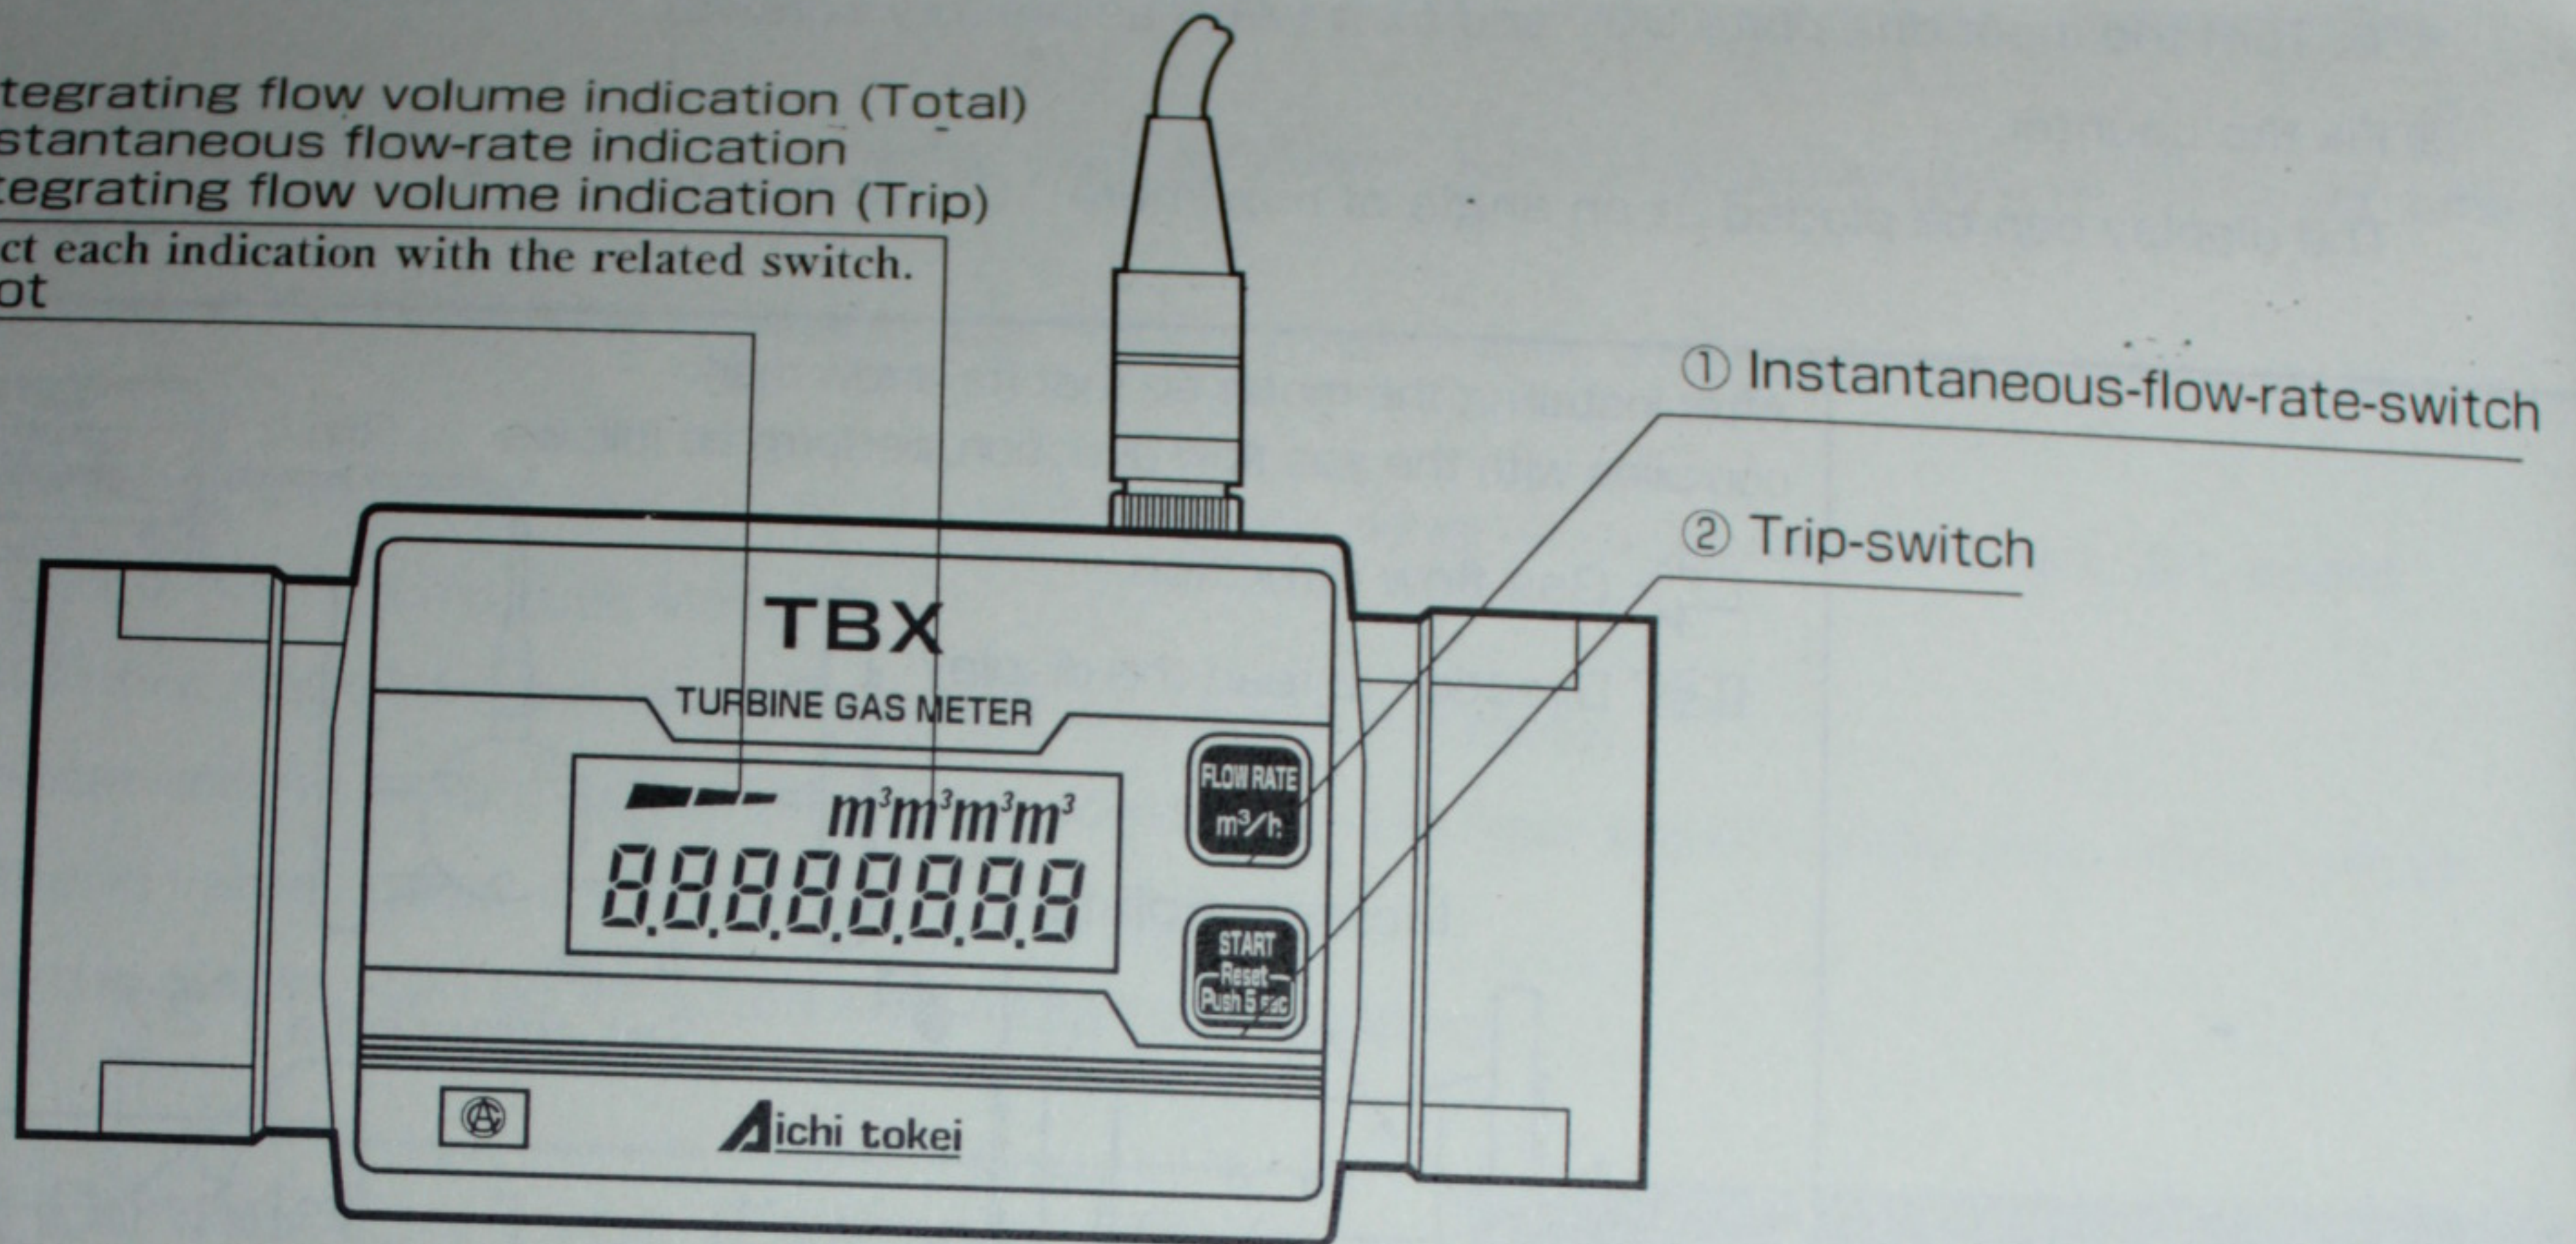



## 2) For TBX150F

- ⑥ Pilot
- ③ Integrating flow volume indication (Total)
- ④ Instantaneous flow-rate indication
- ⑤ Integrating flow volume indication (Trip)
- \* Select each indication with the related switch.

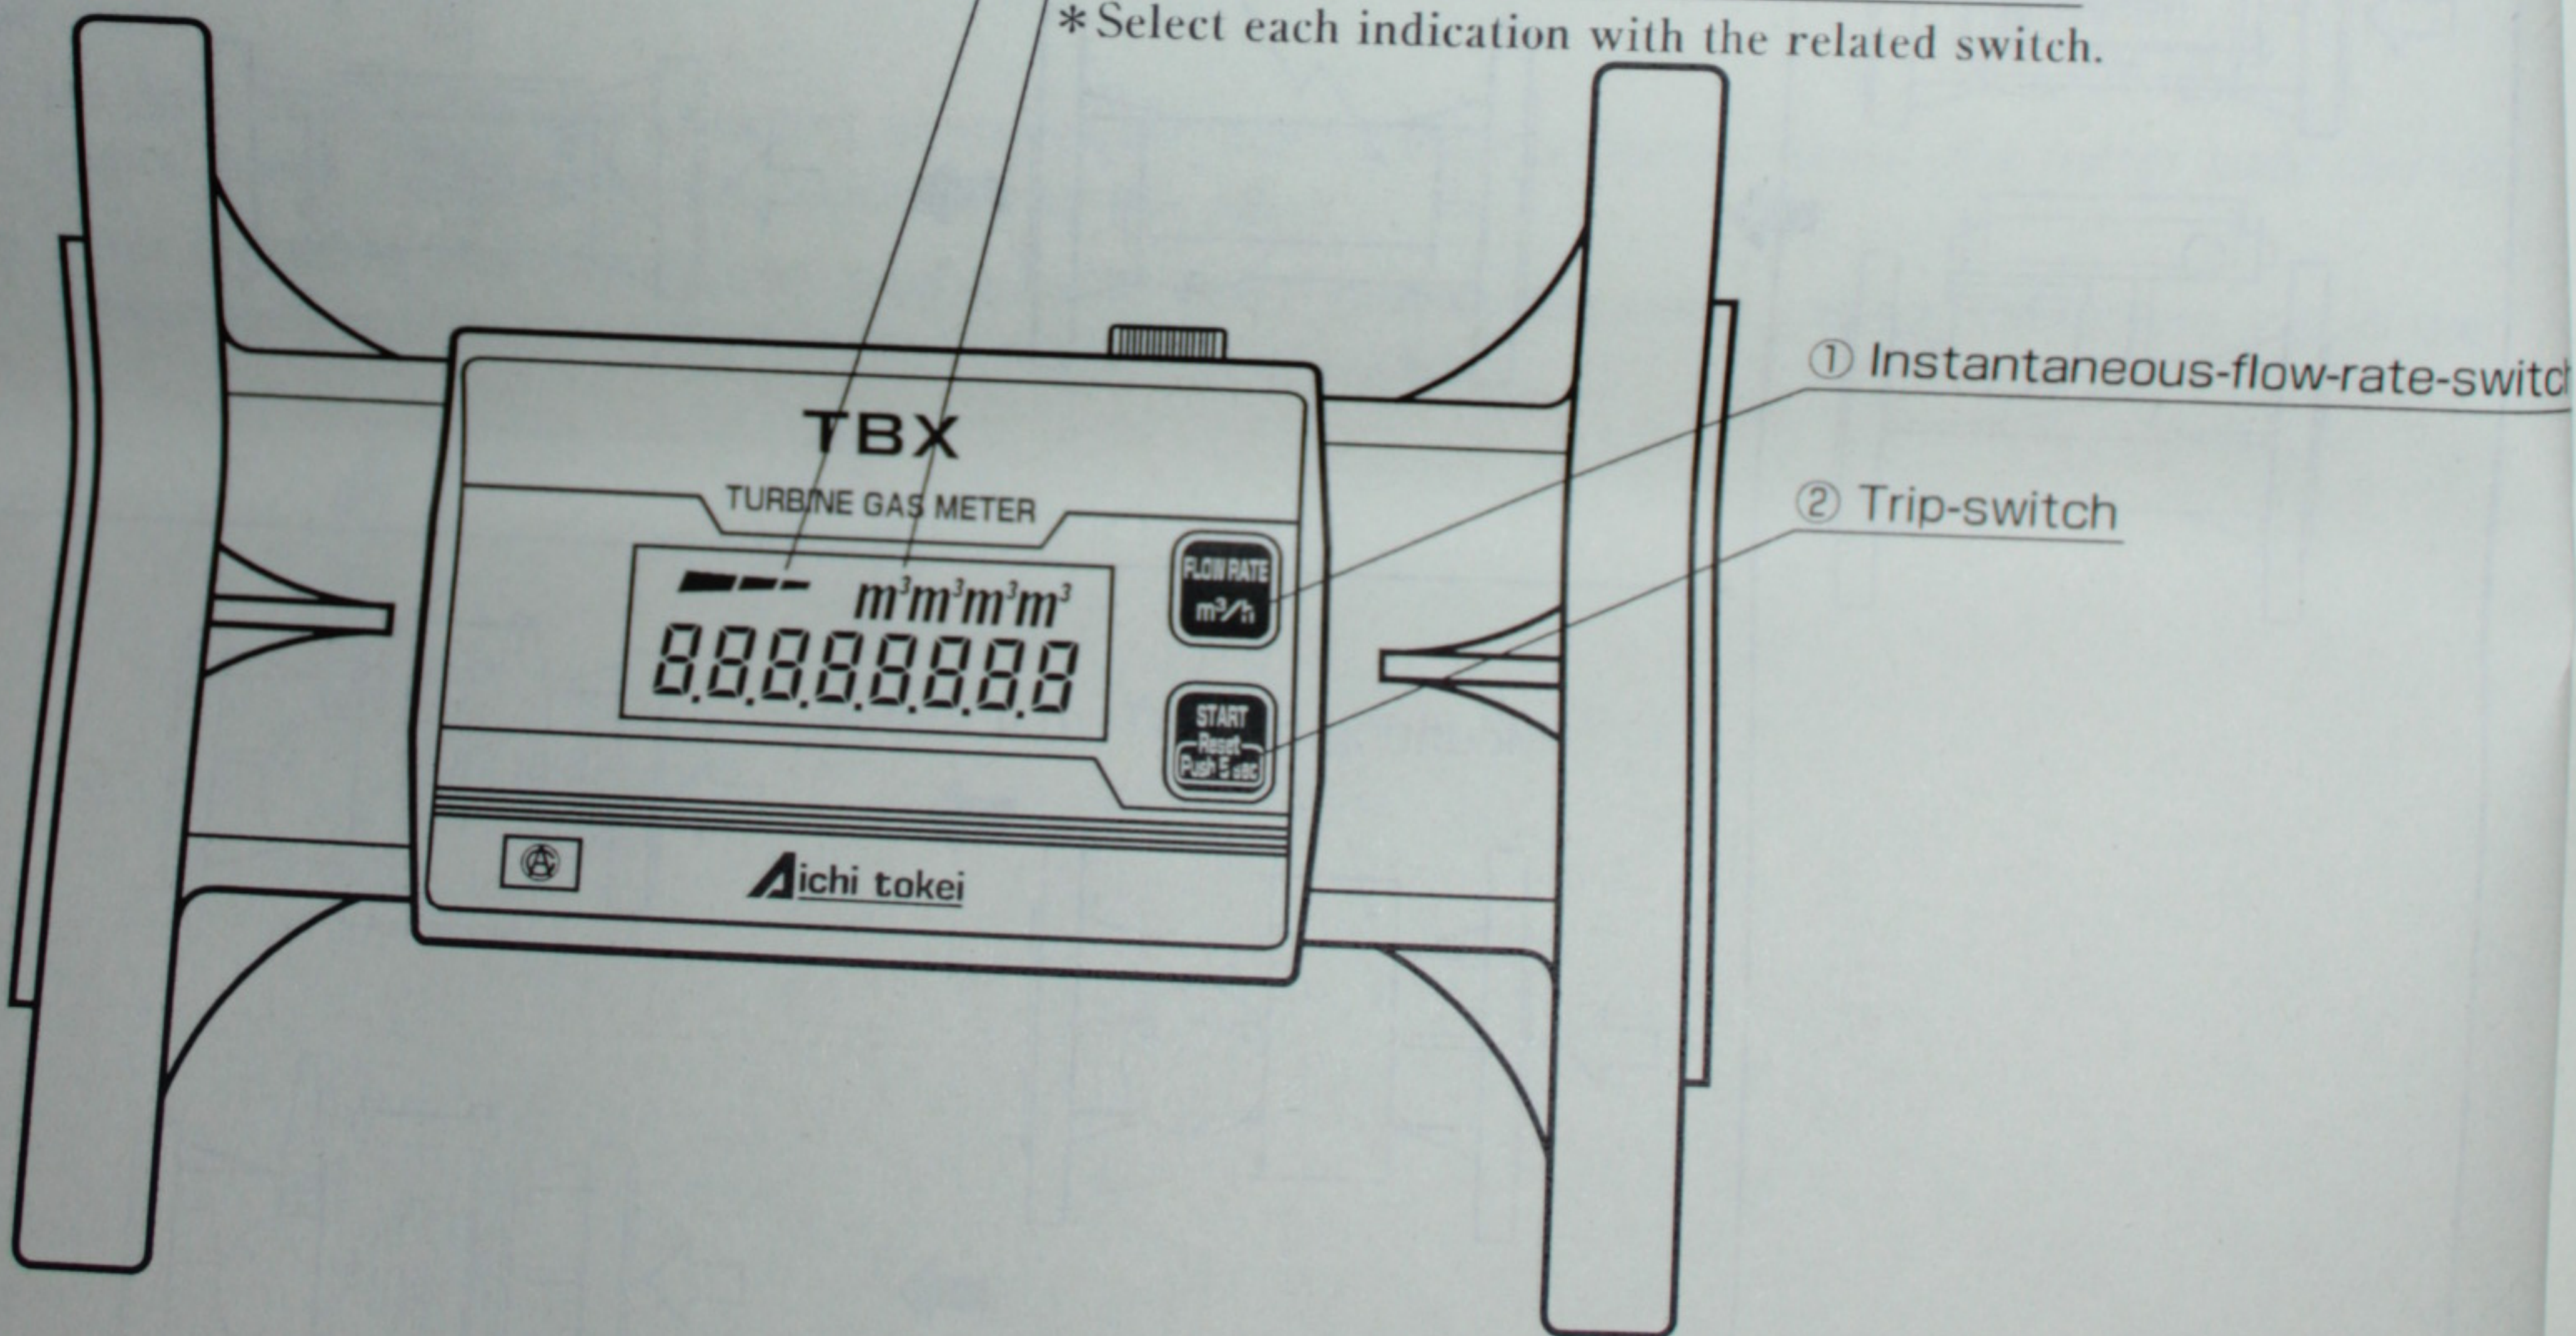

Portion	Model		TBX30	TBX100 TBX100F	TBX150F
	Description				
Switches	①	Instantaneous-flow-rate-switch	<p>[While Integrating Flow Volume (Total) is indicated] Pressing the switch for not more than 1 second indicates Instantaneous Flow-Rate. After 30 seconds since, Integrating Flow Volume (Total) is to be re-indicated automatically.</p> <p>[While Instantaneous Flow-Rate is indicated] Pressing the switch for more than continuous 1 second changeovers the display to the indication which was displayed before the indication of Instantaneous Flow-Rate (Integrating Flow Volume (Total) or Integrating Flow Volume (Trip)). In case of changeover to Integrating Flow Volume (Trip), its value has not been reset.</p> <p>[While Integrating Flow Volume (Trip) is indicated] Pressing the switch for not more than 1 second indicates Instantaneous Flow-Rate. After 30 seconds since, Integrating Flow Volume (Trip) is to be re-indicated automatically.</p>		
	②	Trip-switch	<p>[While Integrating Flow Volume (Total) is indicated] Pressing the switch for not more than 3 seconds indicates flow volume that accumulation is started since (Integrating Flow Volume (Trip)). 5 seconds of continuous pressing changeovers the display back to Integrating Flow Volume (Total).</p> <p>[While Instantaneous Flow-Rate is indicated] Pressing the switch for not more than 3 seconds indicates flow volume that accumulation is started since (Integrating Flow Volume (Trip)).</p> <p>[While Integrating Flow Volume (Trip) is indicated] Pressing the switch for not more than 3 seconds resets the value of Integrating Flow Volume (Trip). Continuous pressing of the switch for 3 seconds or more changeovers the display to Integrating Flow Volume (Total).</p>		
	① + ②	Instantaneous-flow-rate-switch + Trip-switch	<p>[While Integrating Flow Volume (Total) is indicated] Pressing the both switches for continuous 4 seconds or more changeovers the display to the maintenance mode (the pulse constant indication mode). Pressing the both switches for continuous 10 seconds or more changeovers the display to the stock mode.</p> <p>[While Instantaneous Flow-Rate is indicated] Pressing the both switches for continuous 4 seconds or more changeovers the display to the maintenance mode (the pulse constant indication mode). Pressing the both switches for continuous 10 seconds or more changeovers the display to the stock mode.</p> <p>[While Integrating Flow Volume (Trip) is indicated] Pressing the both switches for continuous 4 seconds or more changeovers the display to the maintenance mode (the pulse constant indication mode). Pressing the both switches for continuous 10 seconds or more changeovers the display to the stock mode.</p>		

Portion	Model		TBX30	TBX100 TBX100F	TBX150F
	Description				
Display	③	Integrating flow volume (Total) indication (m <sup>3</sup> )	9999999.99 <sup>m<sup>3</sup></sup>		9999999.9 <sup>m<sup>3</sup></sup>
	④	Instantaneous flow-rate indication (m <sup>3</sup> /h)	u 99.9 <sup>m<sup>3</sup></sup> u	999.9 <sup>m<sup>3</sup></sup>	u 999
	⑤	Integrating flow volume (Trip) indication (m <sup>3</sup> )	9999.99 <sup>m<sup>3</sup></sup>		99999.9 <sup>m<sup>3</sup></sup>
	⑥	Pilot	 Flashing In case gas flows, it indicates the meter is under measuring.		

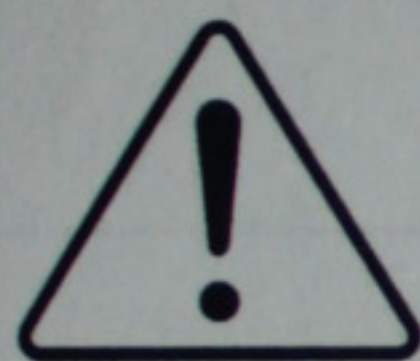

Caution

As pushing the switches strongly with something hard such as a knock pencil, a driver, etc., damages the switches, press them with something soft such as a fingertip.



Do Without Fail

At the time of shipment, the display is protected with the black rubber protector. Do not remove it until the completion of the installation work. In case the meter is to be used at unfavorable ambient environment, leave the protector to cover the display.

### 3) Maintenance mode (Pulse constant indication mode)

While the mode of normal operation (when one of the flow indications is displayed), pressing the both of "Flow-Rate" and "Start (Trip-switch)" switches for continuous 4 seconds or more changeovers the display to this maintenance mode (pulse constant indication mode).

With "Flow-Rate" switch, each item among 5 items can be selected in turn.

At the time of indication of an item to be set (pulse output unit or pulse output width), by pressing "Flow-Rate" switch for continuous 2 seconds or more, setting of the item is started.


By pressing "Flow-Rate" switch, select content of the setting. And, by pressing "Flow-Rate" switch again for continuous 2 seconds or more, the setting is to be settled.

If no operation is performed for 10 seconds or more during indication of any item, or by pressing "Start" switch (Trip-switch), the display is changeover to Integrating Flow Volume (Total).

If no input operation is performed for 10 seconds or more during setting, even though setting is not completed, the display is changeover to Integrating Flow Volume (Total). In the case setting is uncompleted, output pulse setting data to be used is as previous setting value.

Hereunder is the diagram of indication and setting of the items.

Maintenance mode (Pulse constant indication mode): Continuous 4 seconds of "Flow Rate" + "Start" pressing

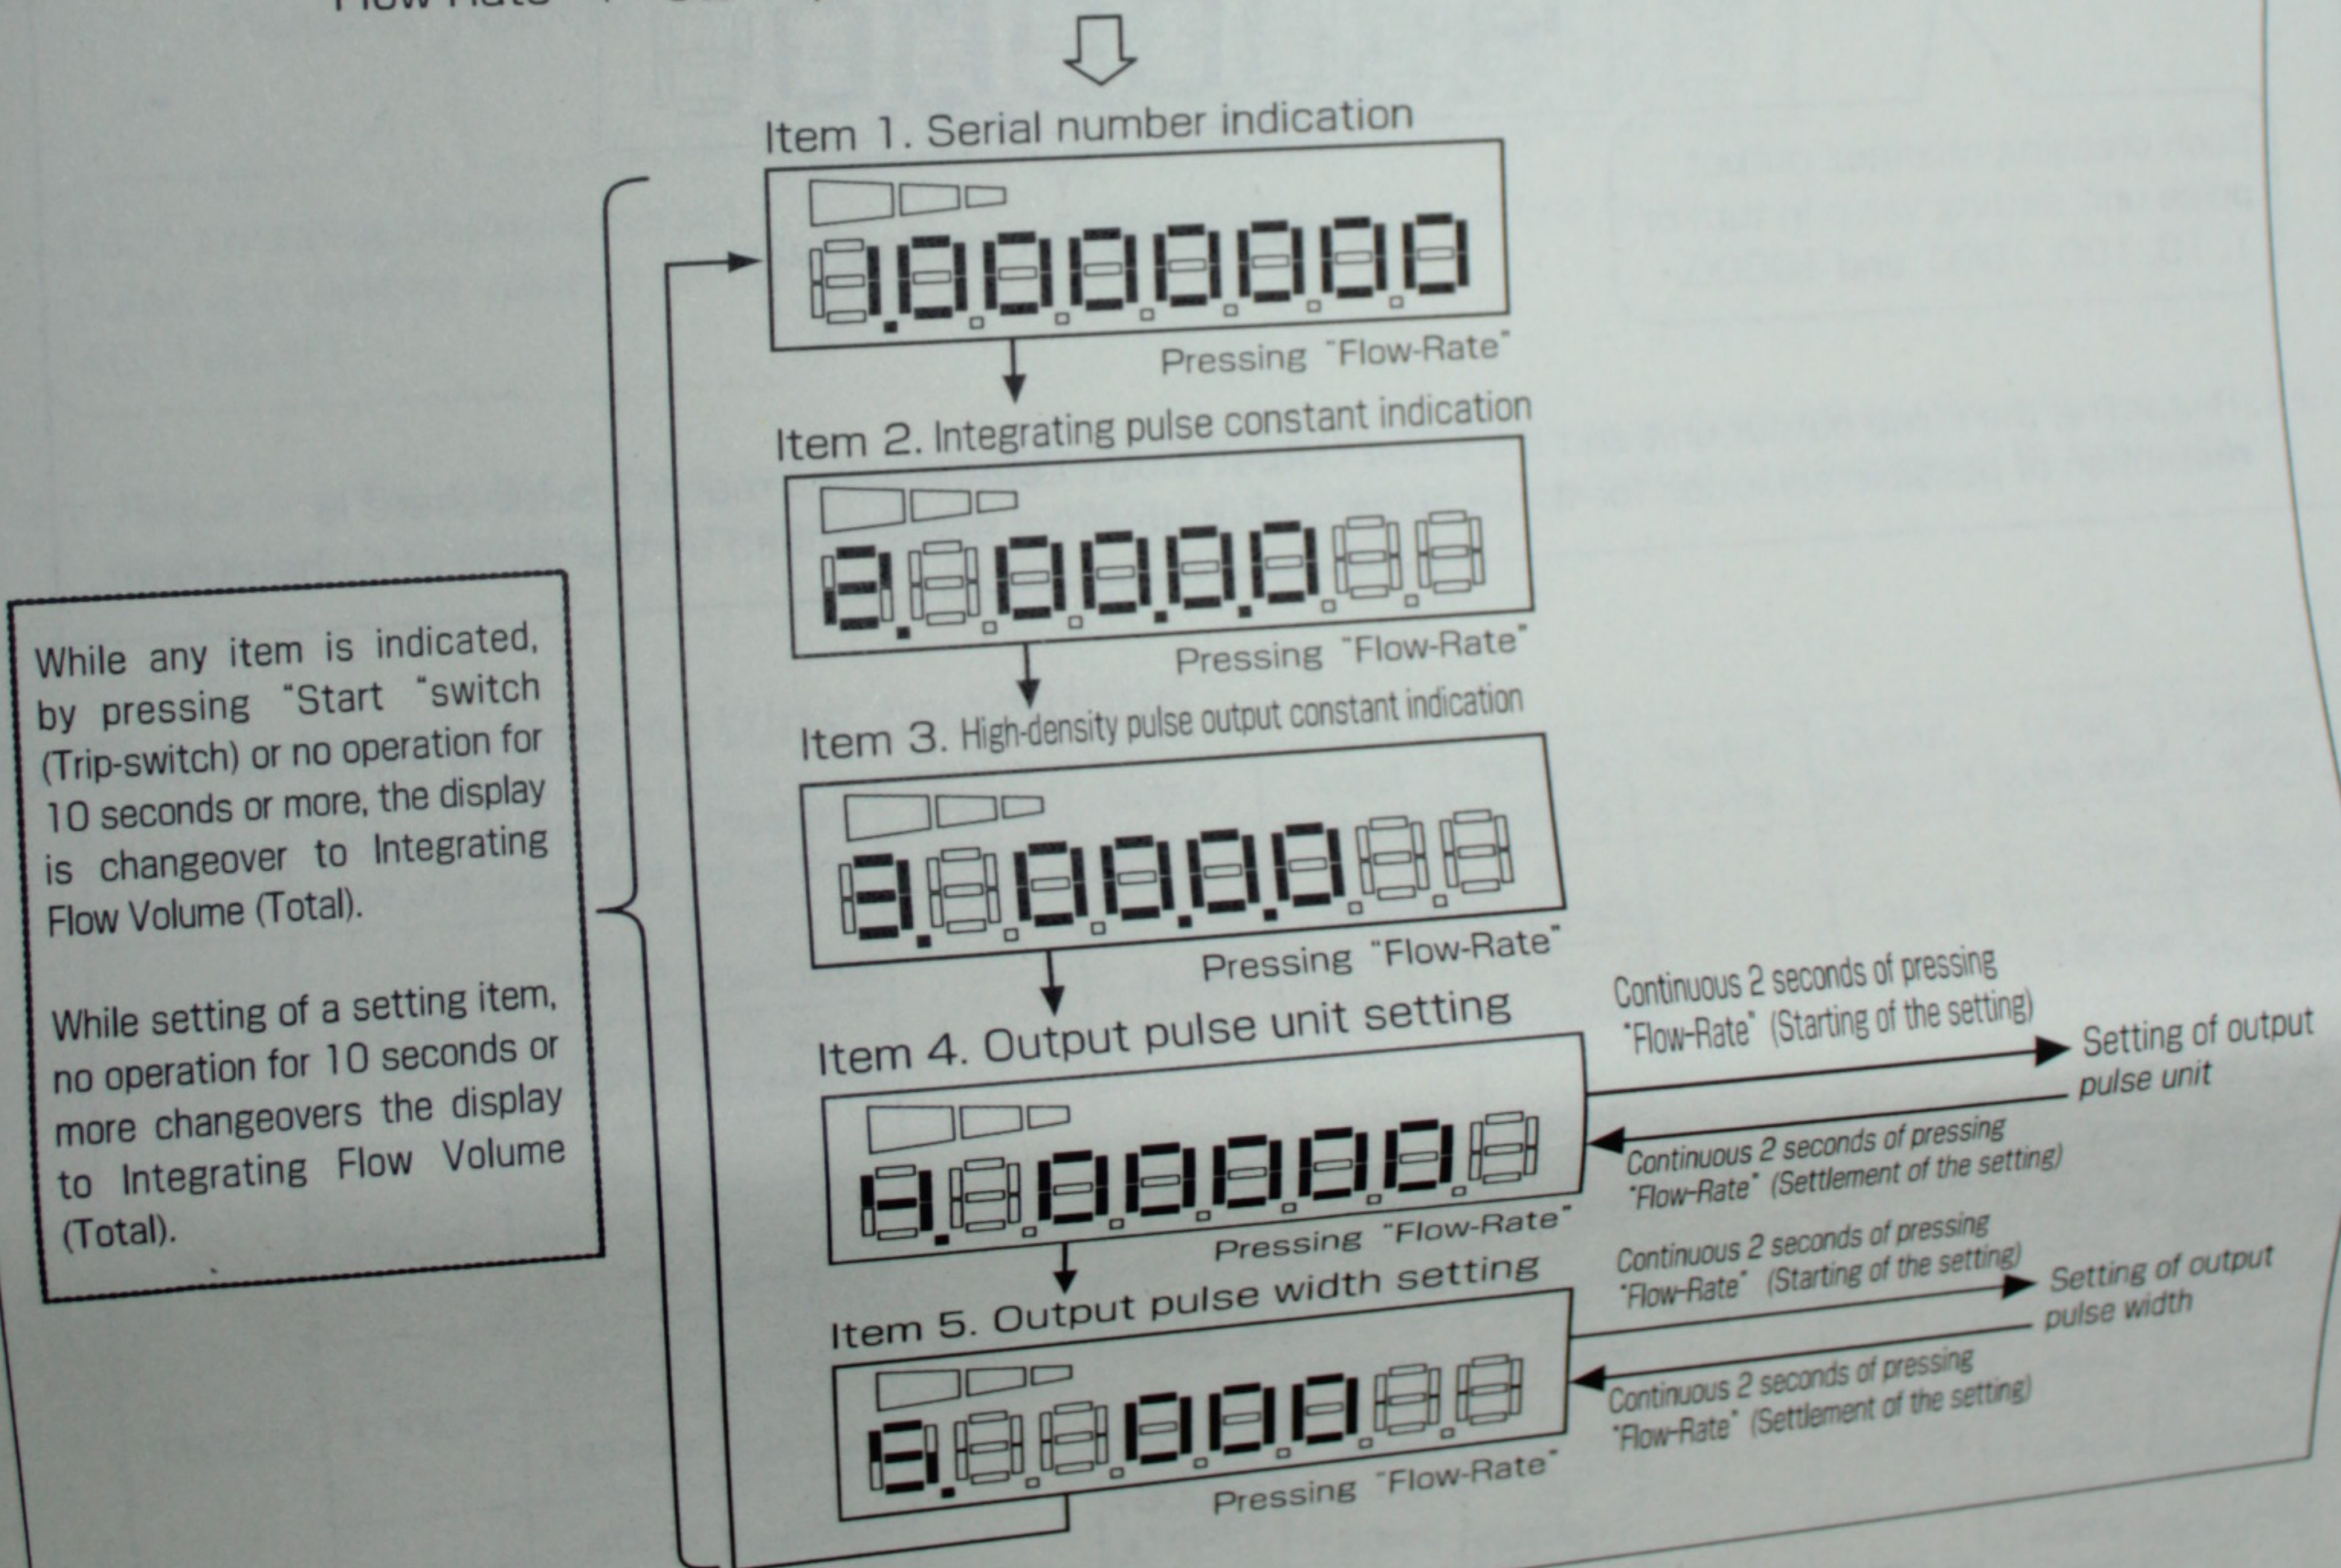

While any item is indicated, by pressing "Start" switch (Trip-switch) or no operation for 10 seconds or more, the display is changeover to Integrating Flow Volume (Total).

While setting of a setting item, no operation for 10 seconds or more changeovers the display to Integrating Flow Volume (Total).

#### 4) Output pulse unit setting

This is the setting of the item no. 4.

By pressing "Flow-Rate" switch for continuous 2 seconds (Starting of the setting), the present setting value of the output pulse unit is flickered (for each 0.5 second).

While flickering of the output pulse unit's setting value, by pressing "Flow-Rate" switch, the setting value is changed within the range of 1~10000L/p (1L/p, 10L/p, 100L/p, 1000L/p (1m<sup>3</sup>/p), 10000L/p (10m<sup>3</sup>/p)).

After the change of the value, pressing "Flow-Rate" switch for continuous 2 seconds settles the setting value (completion of the setting) and the display is changeover to the indication of the item 4 Output pulse unit setting (Indication of the present value).


Hereunder is an image of the setting.

Item 4. Output pulse unit setting (Indication of the present setting value)


Continuous 2 seconds of pressing "Flow-Rate" (Settlement of the setting)

Continuous 2 seconds of pressing "Flow-Rate" (Starting of the setting)

Pressing "Flow-Rate"



Each pressing changes output pulse unit setting value in turn of 1, 10, 100, 1000, and 10000.

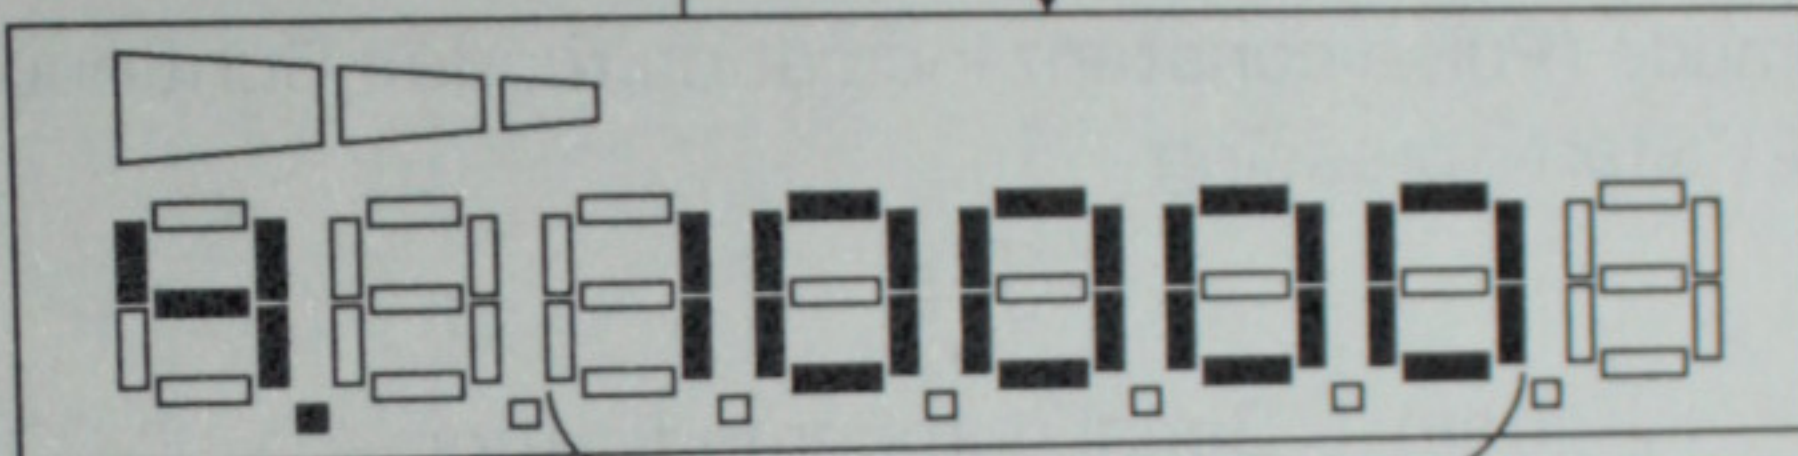

Output pulse unit setting value

※1: Regarding the pulse output unit and the pulse output width, depends on a meter model, there is restriction of possible selection for these pulse output settings as described by the table of 6) hereunder.

## 5) Output pulse width setting


This is the setting of the item no. 5.

By pressing "Flow-Rate" switch for continuous 2 seconds (Starting of the setting), the present setting value of the output pulse width is flickered (for each 0.5 second).

While flickering of the output pulse width's setting value, by pressing "Flow-Rate" switch, the setting value is changed to 40 or 120 in turns. (40ms, 120ms)

After the change of the value, pressing "Flow-Rate" switch for continuous 2 seconds settles the new setting value (completion of the setting) and the display is changeover to the indication of the item 5 Output pulse width setting (Indication of the present value).

Hereunder is an image of the setting.

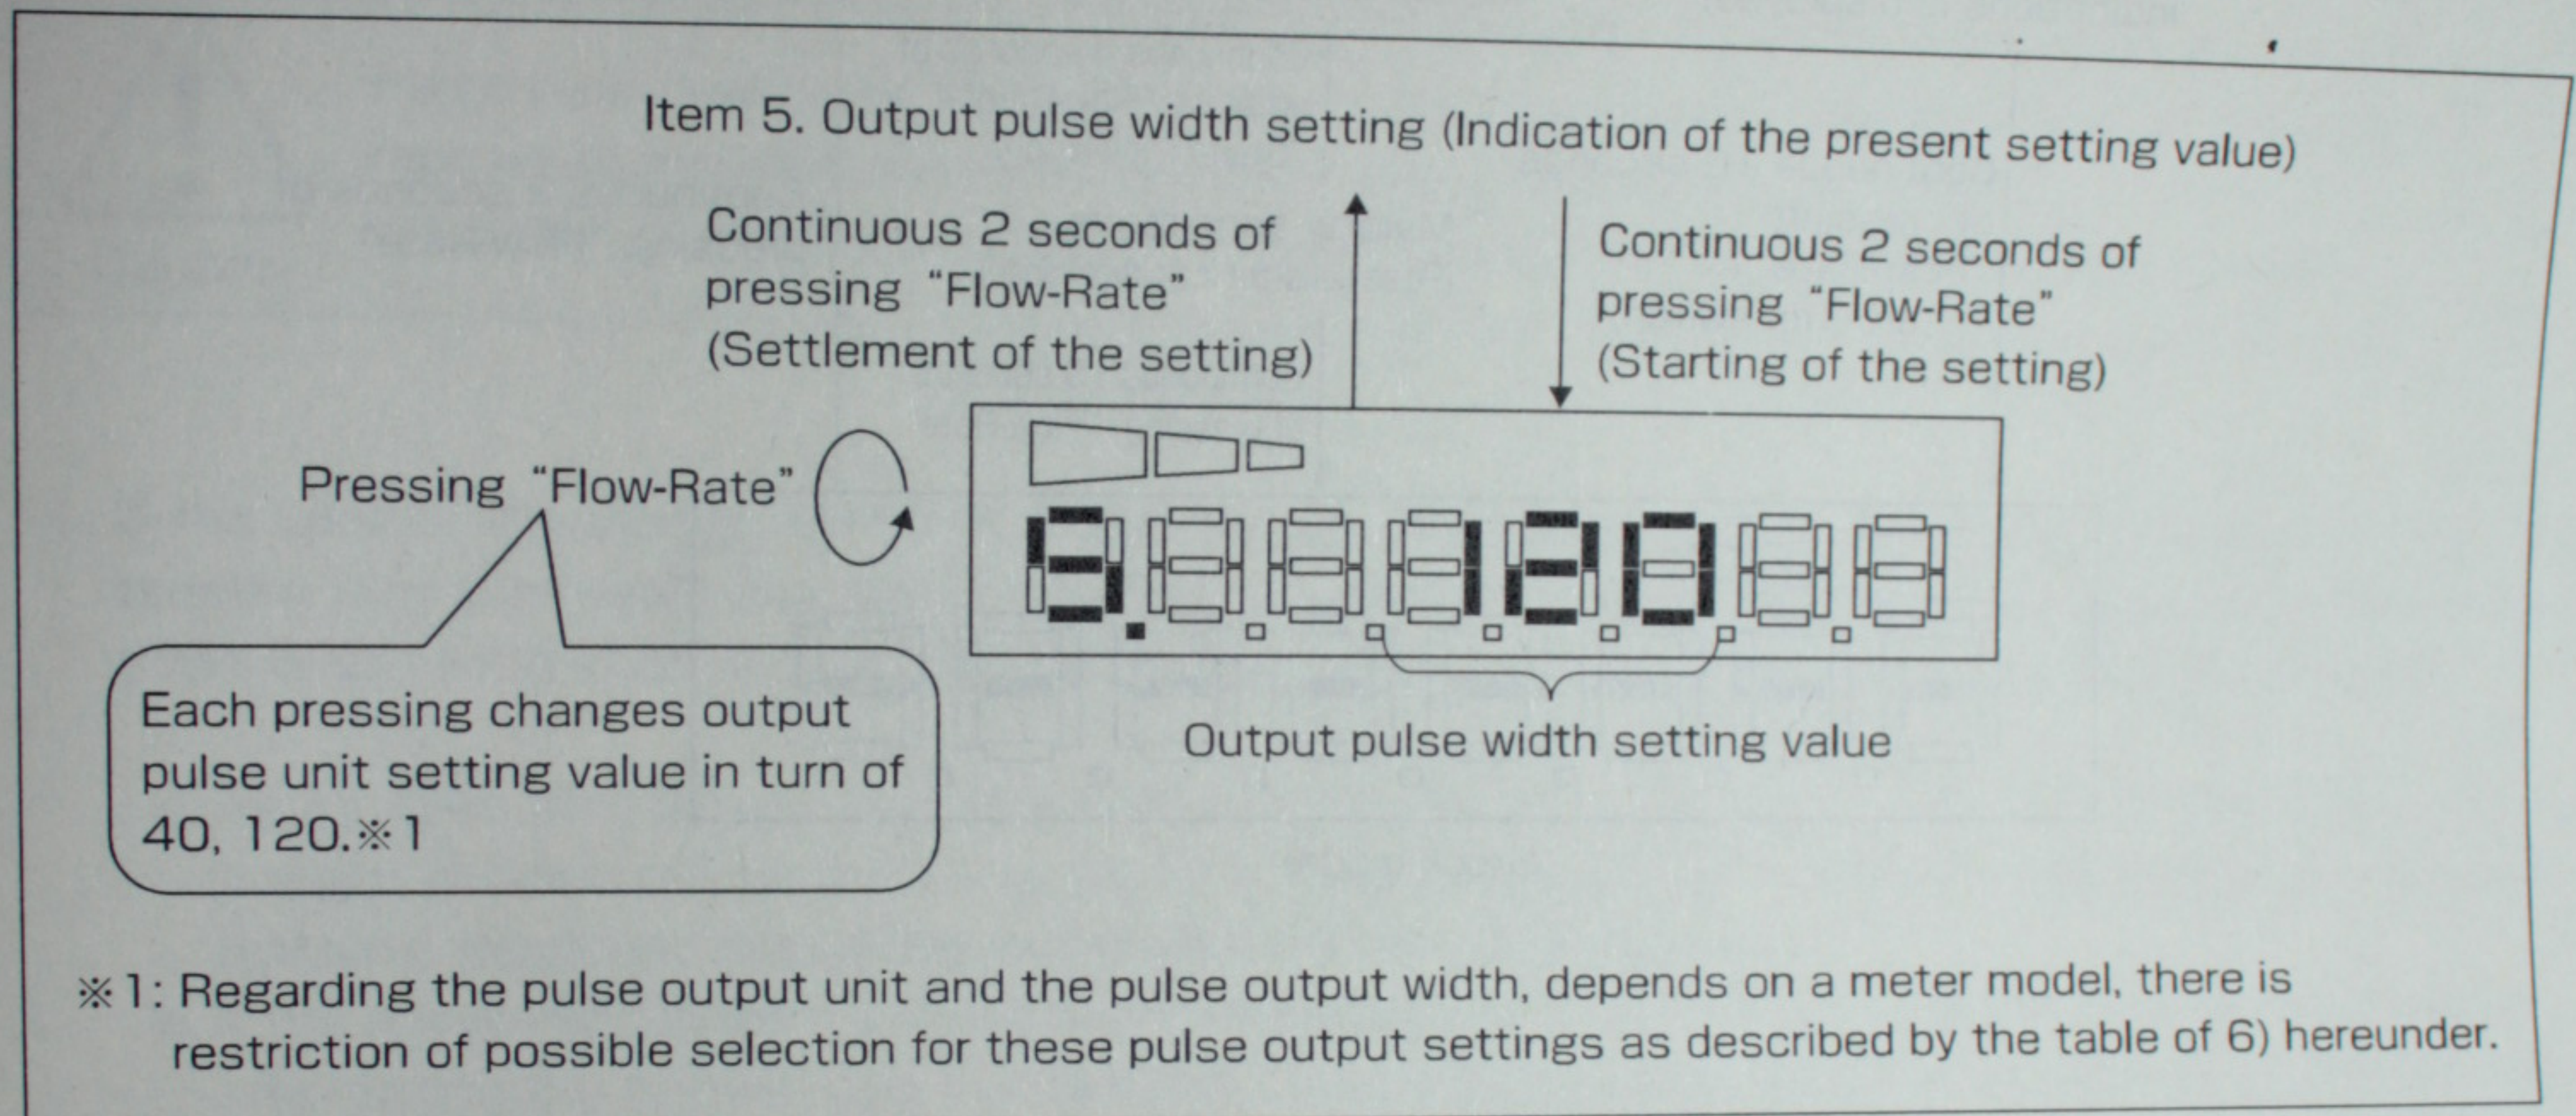

## 6) The output pulse setting conditions

Meter model	Output pulse unit	Output pulse width	Possibility of setting	Meter model	Output pulse unit	Output pulse width	Possibility of setting	Meter model	Output pulse unit	Output pulse width	Possibility of setting
TBX30	1L/P	40ms	○ (Selectable)	TBX 100(F)	1L/P	40ms	× (Not selectable)	TBX 150F	1L/P	40ms	× (Not selectable)
		120ms	× (Not selectable)			120ms	× (Not selectable)			120ms	× (Not selectable)
	10L/P	40ms	○ (Selectable)		10L/P	40ms	○ (Selectable)		10L/P	40ms	○ (Selectable)
		120ms	○ (Selectable)			120ms	○ (Selectable)			120ms	× (Not selectable)
	100L/P	40ms	○ (Selectable)		100L/P	40ms	○ (Selectable)		100L/P	40ms	○ (Selectable)
		120ms	○ (Selectable)			120ms	○ (Selectable)			120ms	○ (Selectable)
	1000L/P (1m <sup>3</sup> /P)	40ms	○ (Selectable)		1000L/P (1m <sup>3</sup> /P)	40ms	○ (Selectable)		1000L/P (1m <sup>3</sup> /P)	40ms	○ (Selectable)
		120ms	○ (Selectable)			120ms	○ (Selectable)			120ms	○ (Selectable)
	10000L/P (10m <sup>3</sup> /P)	40ms	○ (Selectable)		10000L/P (10m <sup>3</sup> /P)	40ms	○ (Selectable)		10000L/P (10m <sup>3</sup> /P)	40ms	○ (Selectable)
		120ms	○ (Selectable)			120ms	○ (Selectable)			120ms	○ (Selectable)


## 7) Stock mode

To minimize battery consumption during stock, this stock mode is provided.

During the stock mode, the LCD shows "-----".

Integration of flow volume and pulse output are not performed.


The operation method for changeover to the stock mode and from the stock mode to the normal operation mode is as mentioned hereunder.

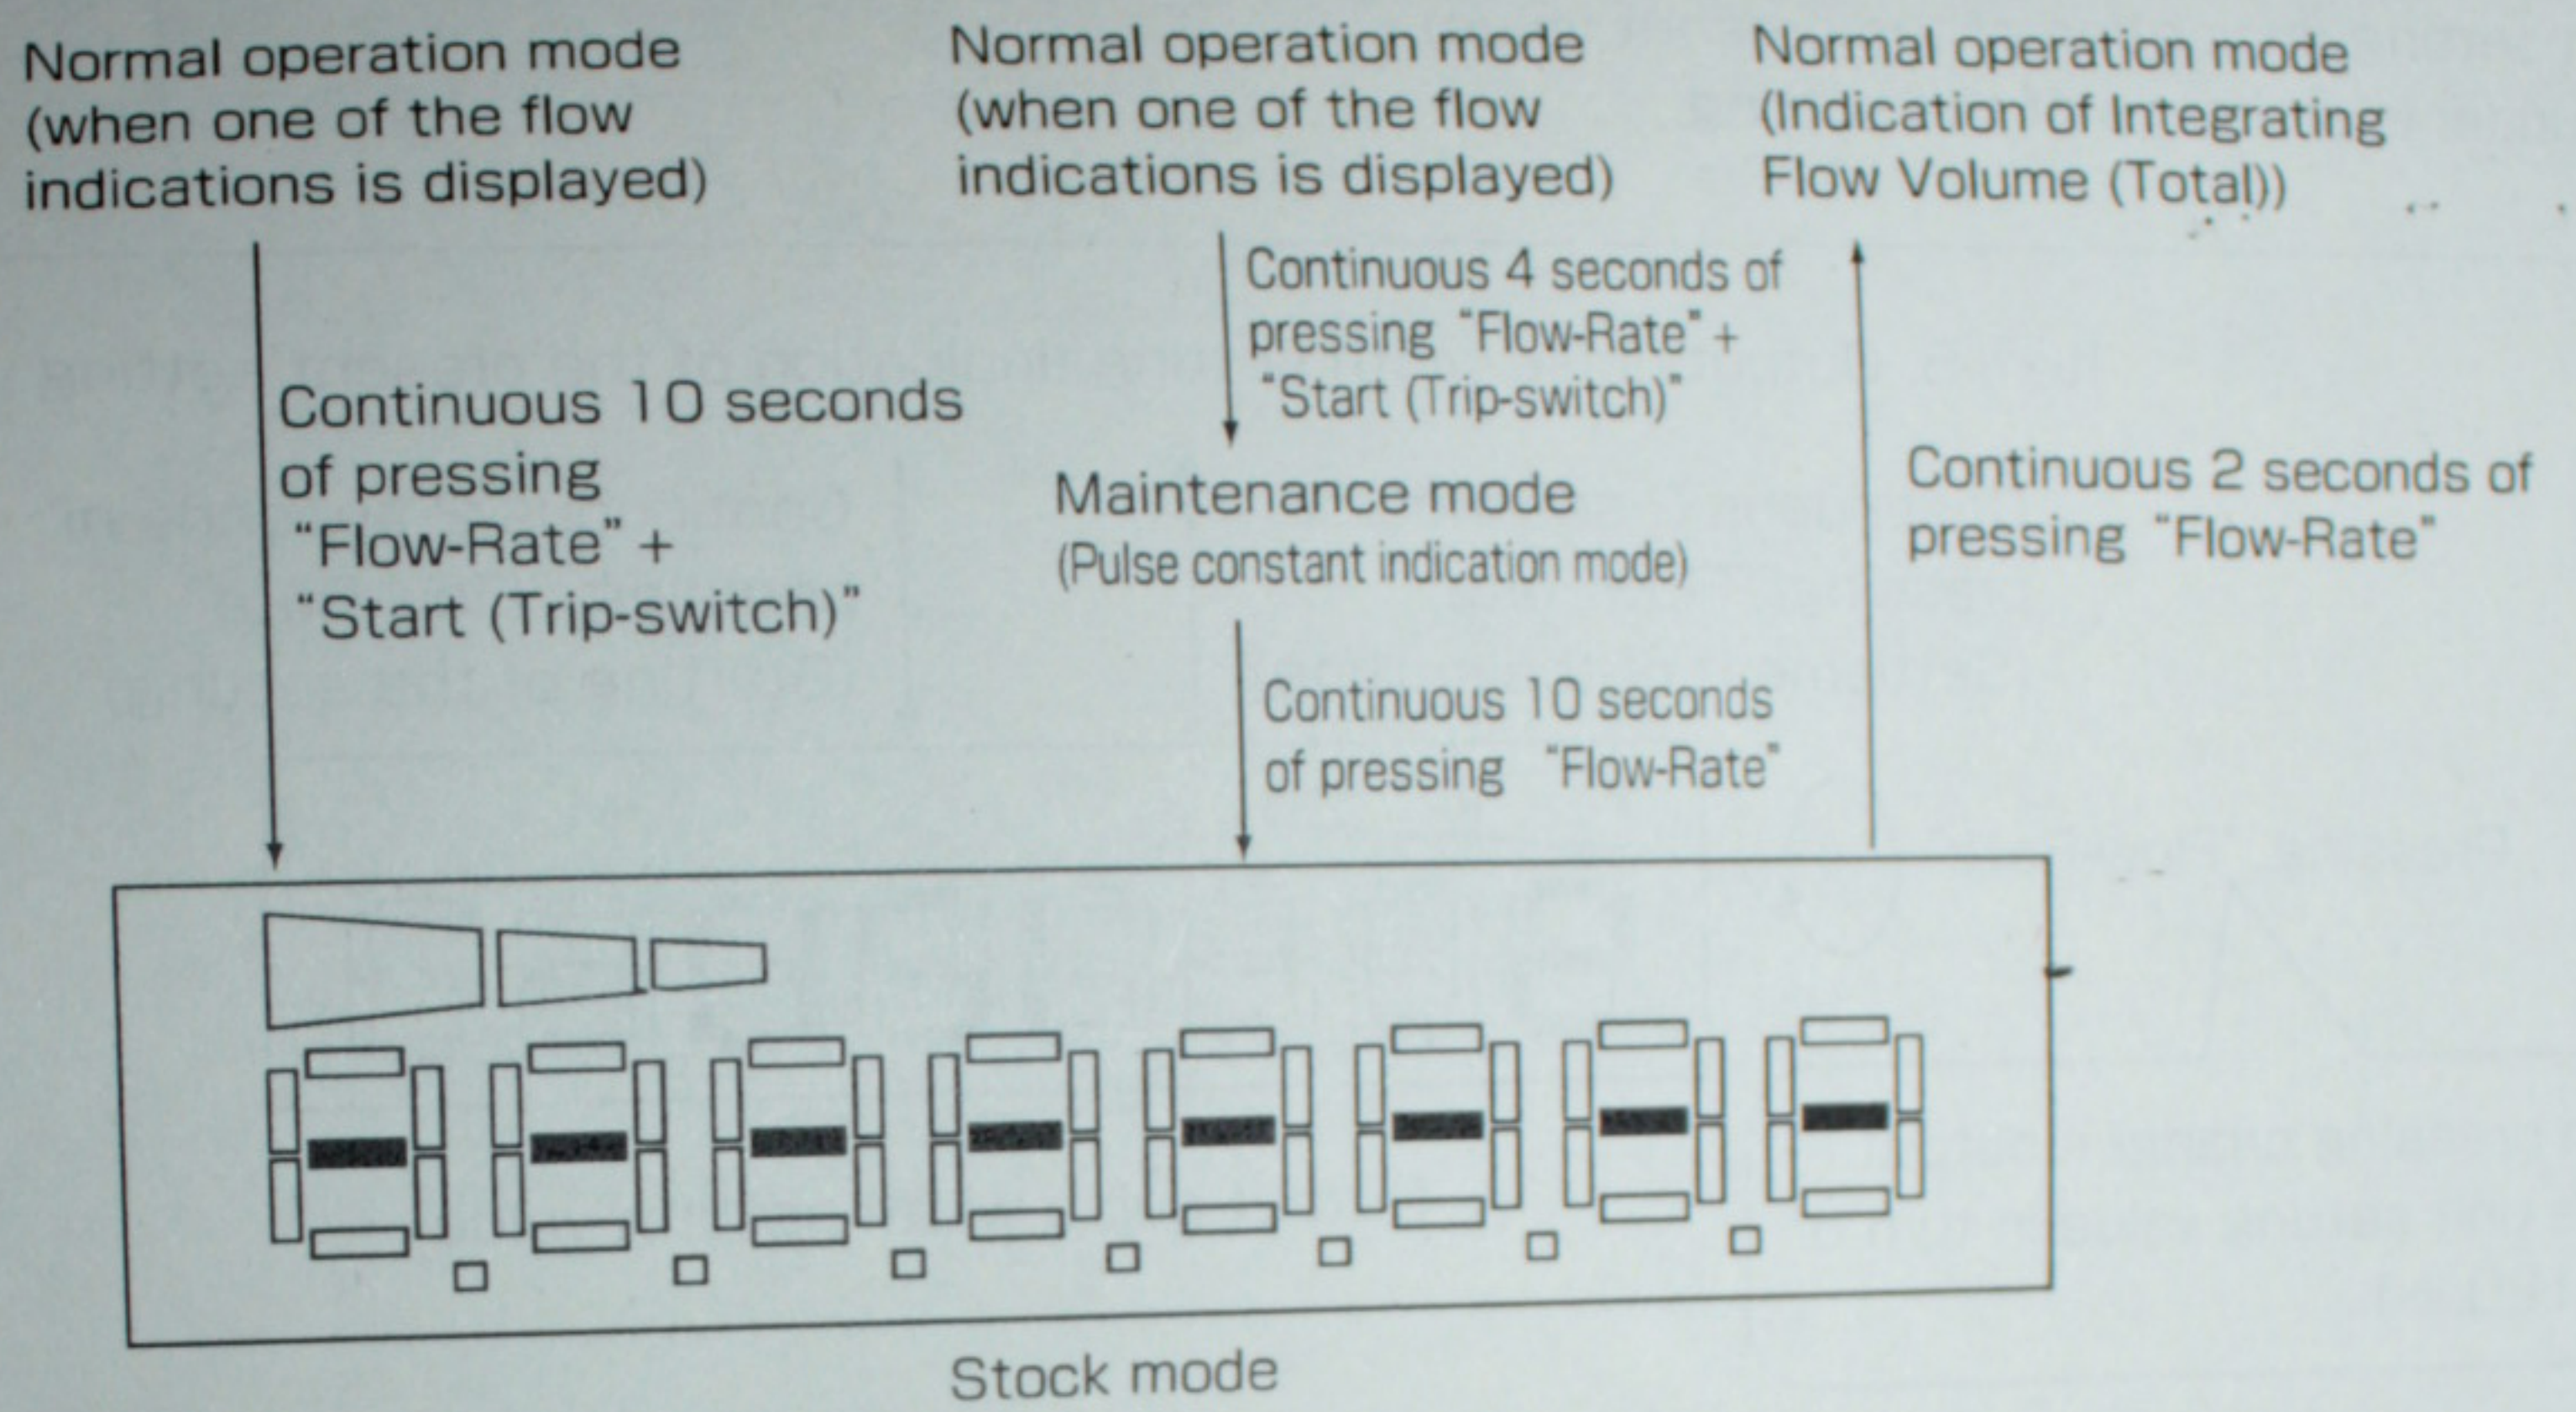

## 6. STARTING OPERATION PROCEDURE

1. Gradually open a valve at inlet side (at upstream of the meter).
2. Gradually open a valve at outlet side (at downstream of the meter).  
Confirm flashing of the pilot.
3. Switch the indication of the meter to instantaneous flow-rate indication and set flow-rate to that of requirement with valve adjustment.
4. Switch the indication to the normal condition, which is integrating flow volume (Total) indication, and utilize the meter under the condition.

## 7. INSPECTION PROCEDURE

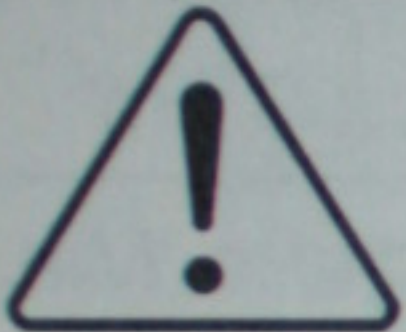

Caution

Rapid deterioration of the meter performance may happen depends on kind of gas to be measured, installation environment(s), and/or working condition(s).  
Execution of periodical inspection suitable to your working conditions is necessary.

1. If the pilot of the display does not flicker though gas flows, remove the meter from piping. Then, lightly breathe into the meter and check whether the pilot flickers. In case the pilot does not flicker, check if there is any adherence of dust, etc., inside the meter and remove the same as occasion demands.
  - a. As for dust, etc., around the outer portion of the turbine rotor, there is possibility that giving the meter a slight shock removes the same. (As the meter is a precision measuring instrument, giving the meter a strong shock and hitting the meter with a thing are prohibited.)
  - b. If the above-mentioned a. cannot be the solution, please put the following measures into practice.
    - By holding the turbine rotor with a finger not to rotate, apply factory air to blow away the dust, etc.
    - Remove the dust, etc., with tweezers or a sharp pointed tool.
  - c. In case seal-material is adhered and removing the same is not possible at a worksite nevertheless the above-mentioned measures, as recovering to the original state is not available from the structural reason, please replace with the new one.
2. After the removal of dust, etc., lightly breath into the meter again. And, if the pilot flickers, it is the evidence of recovery to normal.
3. In case the utmost digit of integrating flow volume indication flickers, it is the alarm of run-out of battery. Urgent replacement of the meter is recommended.





# 8. SPECIFICATIONS

Model		TBX30	TBX100	TBX100F	TBX150F
Description					
Flow range (m <sup>3</sup> /h)		4~30	10~100	10~100	12.5~150
Max. Working Pressure (kPa)		100			
Accuracy		± 1%FS			
Display	Integrating (Total)	LCD 8 digits, Min. reading 10L			LCD 8 digits, Min. reading 0.1 m <sup>3</sup>
	Integrating (Trip)	LCD 6 digits, Min. reading 10L			LCD 6 digits, Min. reading 0.1 m <sup>3</sup>
	Instantaneous	LCD 3 digits, Min. reading 0.1 m <sup>3</sup> /h	LCD 4 digits, Min. reading 0.1 m <sup>3</sup> /h		LCD 3 digits, Min. reading 1 m <sup>3</sup> /h
Gas flow direction (Selectable)		Left to right (L) Right to left (R)	Left to right (L) Right to left (R)	Left to right (L), Right to left (R) Upward, Downward	Left to right (L) Right to left (R)
Connection (Selectable for TBX30)		Rc 1 1/2 , Rc 1 1/4	Rc 2	2BFlange (JIS10K)	
Working temperature range (°C)		-10~60			
Position of installation		Horizontal / vertical			
Kind of gas to be measured		City gas*1, Natural gas*1, LP gas*1, air, nitrogen, etc.			
Power supply		Built-in lithium battery			
Output signal		Open-drain output × 2 (Unit pulse, high density pulse)			
Place to be installed		Indoor			
Material		Aluminum alloy		Cast iron	Aluminum alloy
Weight (kg)		0.8	1.8	7.0	2.5




\* 1: As for measuring LP gas, city gas, or natural gas, please avoid installing the meter in a place where carbide substance (C5 or above) and/or dust powder, etc., waft.

## 9. DIMENSIONS

TBX30 (TBX100)

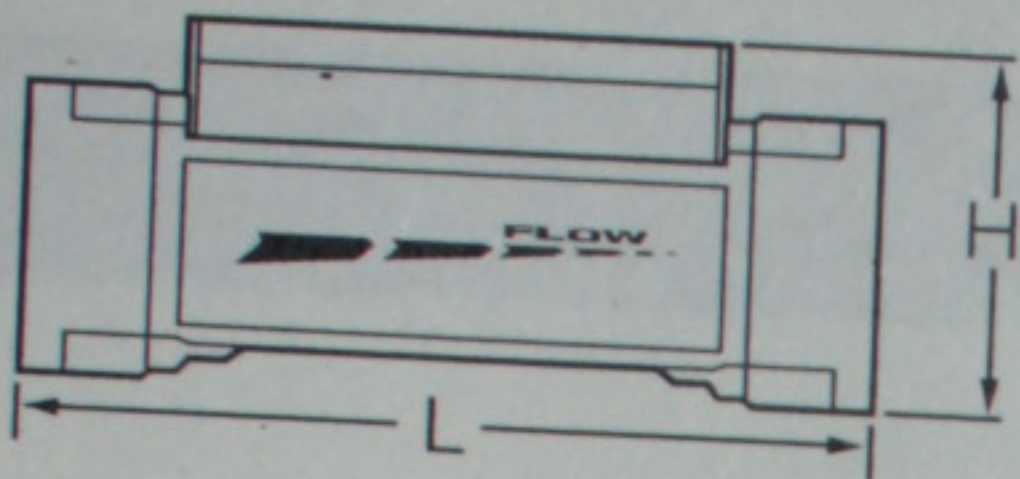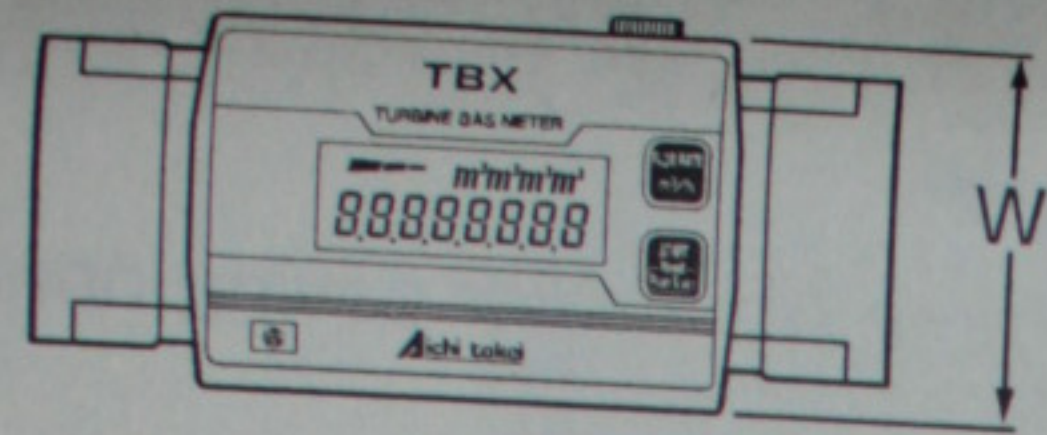



TBX100F (TBX150F)

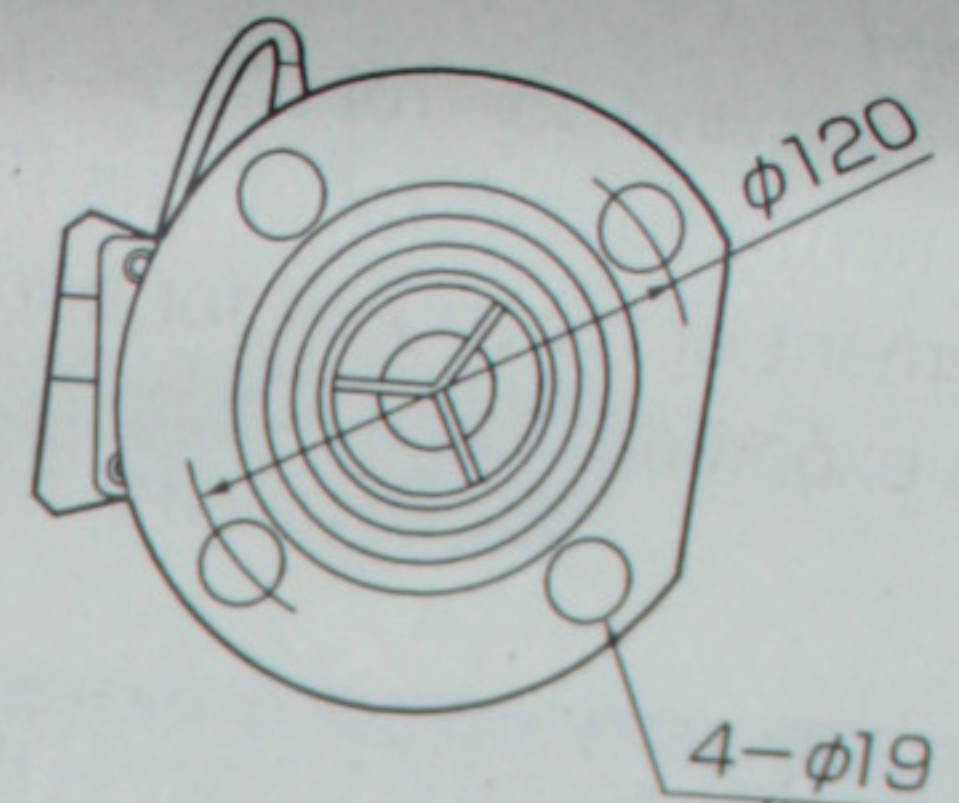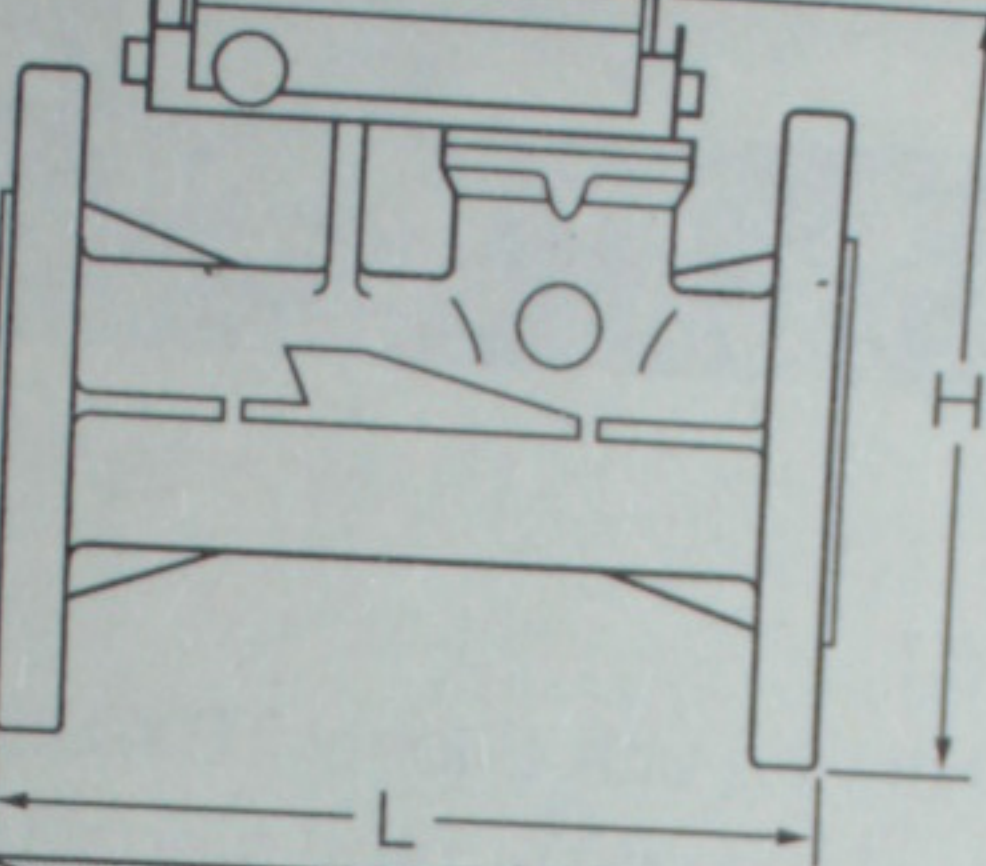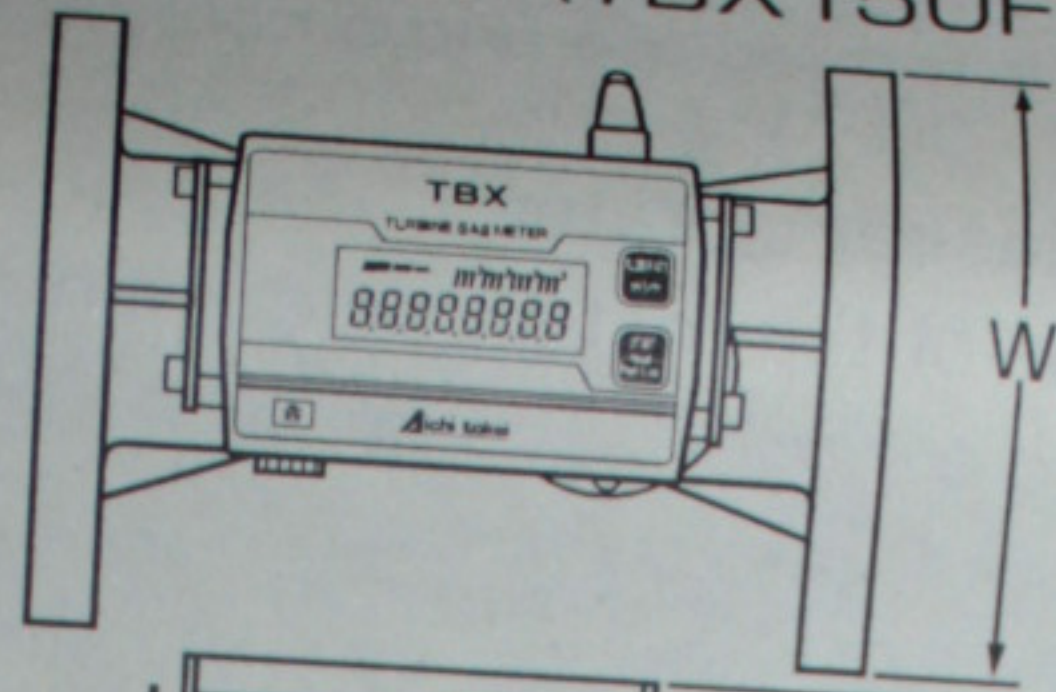

The display of TBX100F may be positioned in any direction so as to match with the flow direction of gas. In addition, the display can be removed and utilized as the remote display.

Model	Dimension		
	L	H	W
TBX30	170	74	73
TBX100	200	100	85
TBX100F	200	161	φ155
TBX150F	200	148	φ155

## 10. SERVICE LIFE

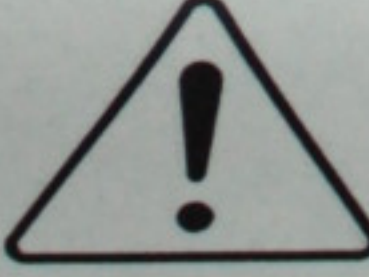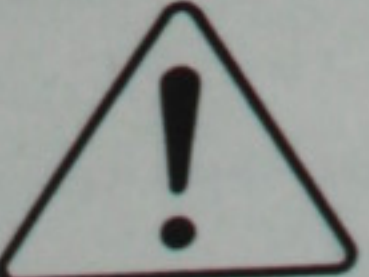Description	Standard service life	Note
Main body of the Turbine Gas Meter	7 years	 Caution In case of flow of oil mist and/or dust powder, etc., inside piping or of continuous long time use at flow-rate exceeding the maximum flow-rate, the service life is to be shorter.
Lithium battery	7 years	 Caution Continuous use at high temperature environment (60°C or higher) shorter the service life.

Note 1) For all the TBX models  
 There is the alarm function to inform within approx. 1 month of run-out-of-battery, with flickering the utmost digit of the integrating flow volume indication.

# 11. APPLICATION EXAMPLES

The meter can be applied for flow managements / controls as follows.

- Management and control of gas flow of a combustion equipment such as a burner, a boiler, a furnace, etc.
- Management and control of gas flow of an intermediate and a compact size water-cooling and -heating equipment.
- Management and control of gas flow of a gas-refrigerator.
- Management and control of gas flow as one of the factory instrumentation.
- Management of factory air for each line and control of compressor running time (as power saving operation).
- Various experiment apparatus in which flow of gas is involved.

# 12. OUTPUT SIGNAL

This meter has 2-circuits of open-drain output (\*1).

For the output signals, utilize the exclusive signal wire unit (Model TBX-SS-B).

After fixing the solderless terminals (Accessory of the unit) to the signal wires, connect them to the terminal box.

## Standard specification

Model	Unit pulse			High density pulse		Maximum impressed voltage
	Pulse unit	Pulse width	Maximum ON resistant(*2)	Pulse unit	Maximum ON resistant(*2)	
TBX30	0.01 m <sup>3</sup> /p	40ms	50Ω	Approx. 110 cm <sup>3</sup> /p *2	100Ω	24V·DC
TBX100				Approx. 250 cm <sup>3</sup> /p *3		
TBX100F				Approx. 250 cm <sup>3</sup> /p *4		
TBX150F	0.10 m <sup>3</sup> /p	Approx. 470 cm <sup>3</sup> /p *5				

\*1: Unit pulse: Flow pulse which unit is settled to the certain pulse unit by the calculation circuit.

High density pulse: Actual flow pulse of which signal output synchronizes with rotation of the turbine rotor.

\*2: Off resistance is 100kΩ or more.

# 13. SIGNAL WIRE UNIT (OPTION)

TBX-SS-B


The signal wire unit is to connect the meter with a remote display, a counter, etc., which is consisted of signal wire with the plug and the terminal box to replay signals.




Signal wire (2m) with plug

## Connection method to utilize output signal

Kind of flow pulse	Unit pulse		High density pulse	
Color of signal wires	Red	Blue	White	Black
Polarity of terminals	+	-	+	-

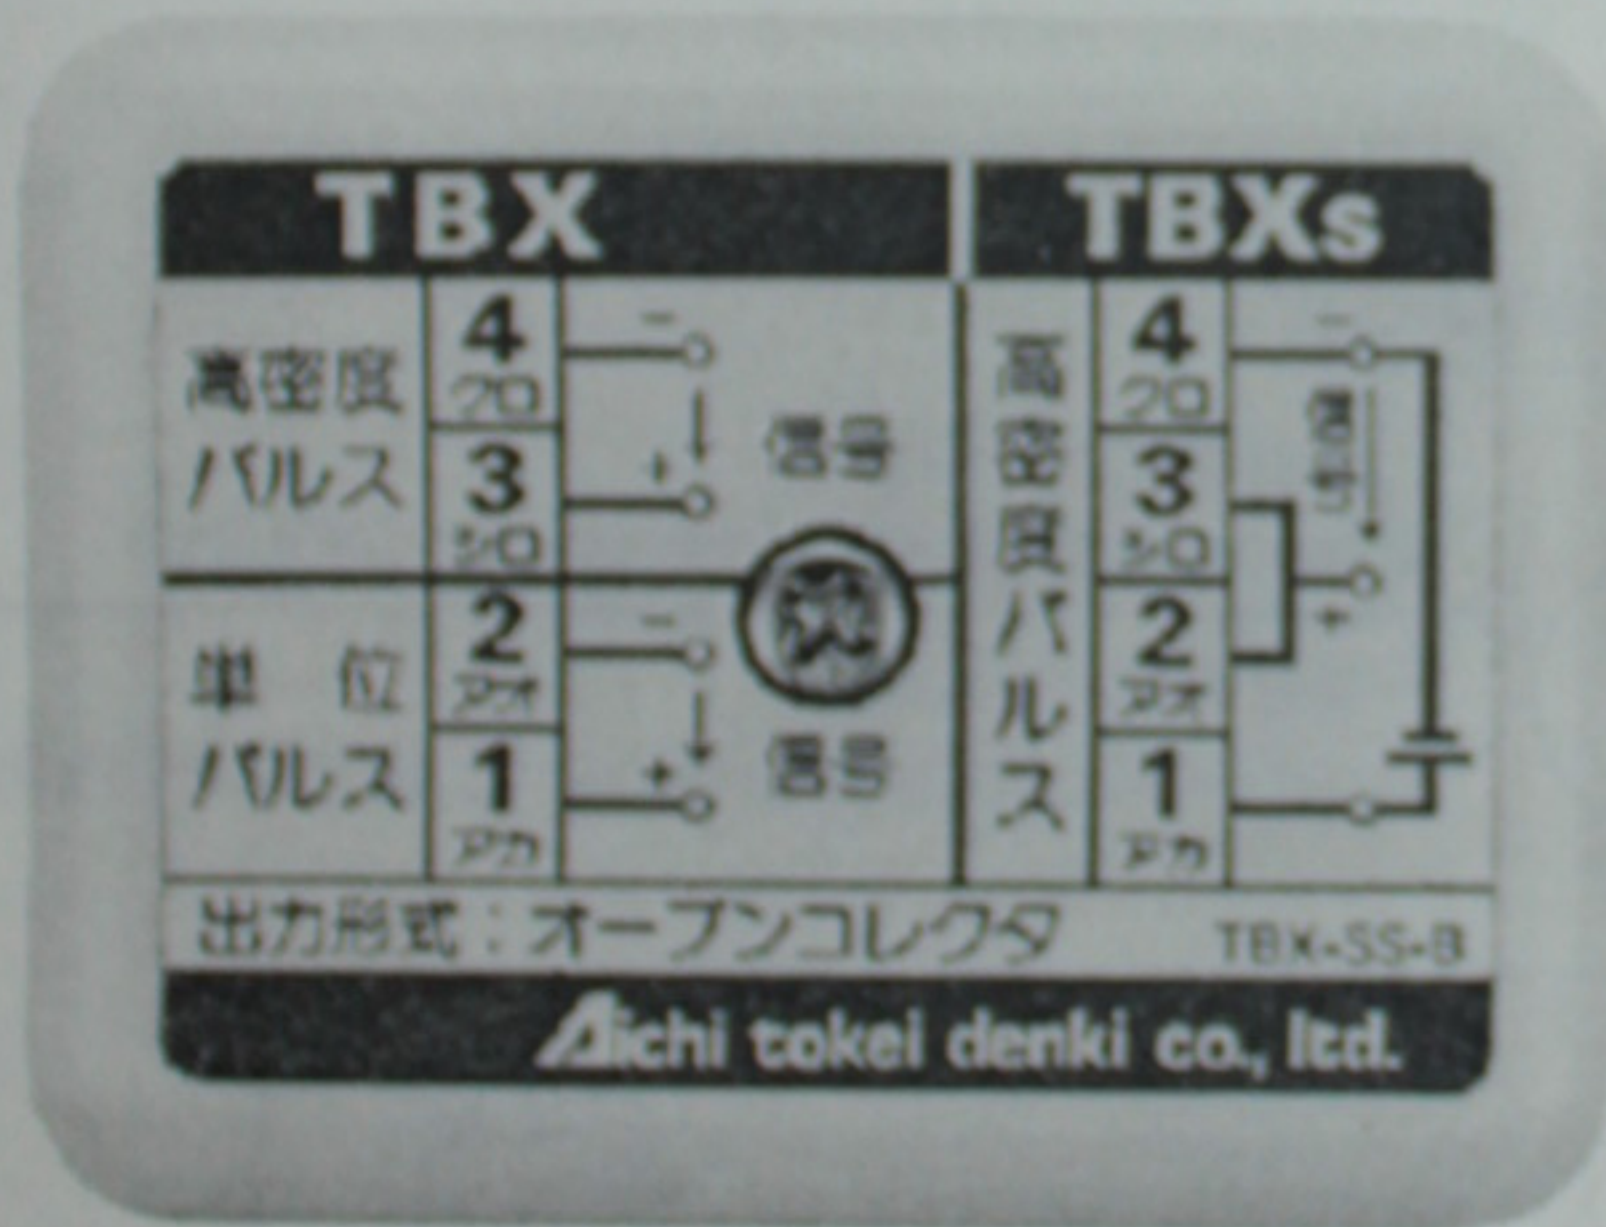

Terminal box (Outside)

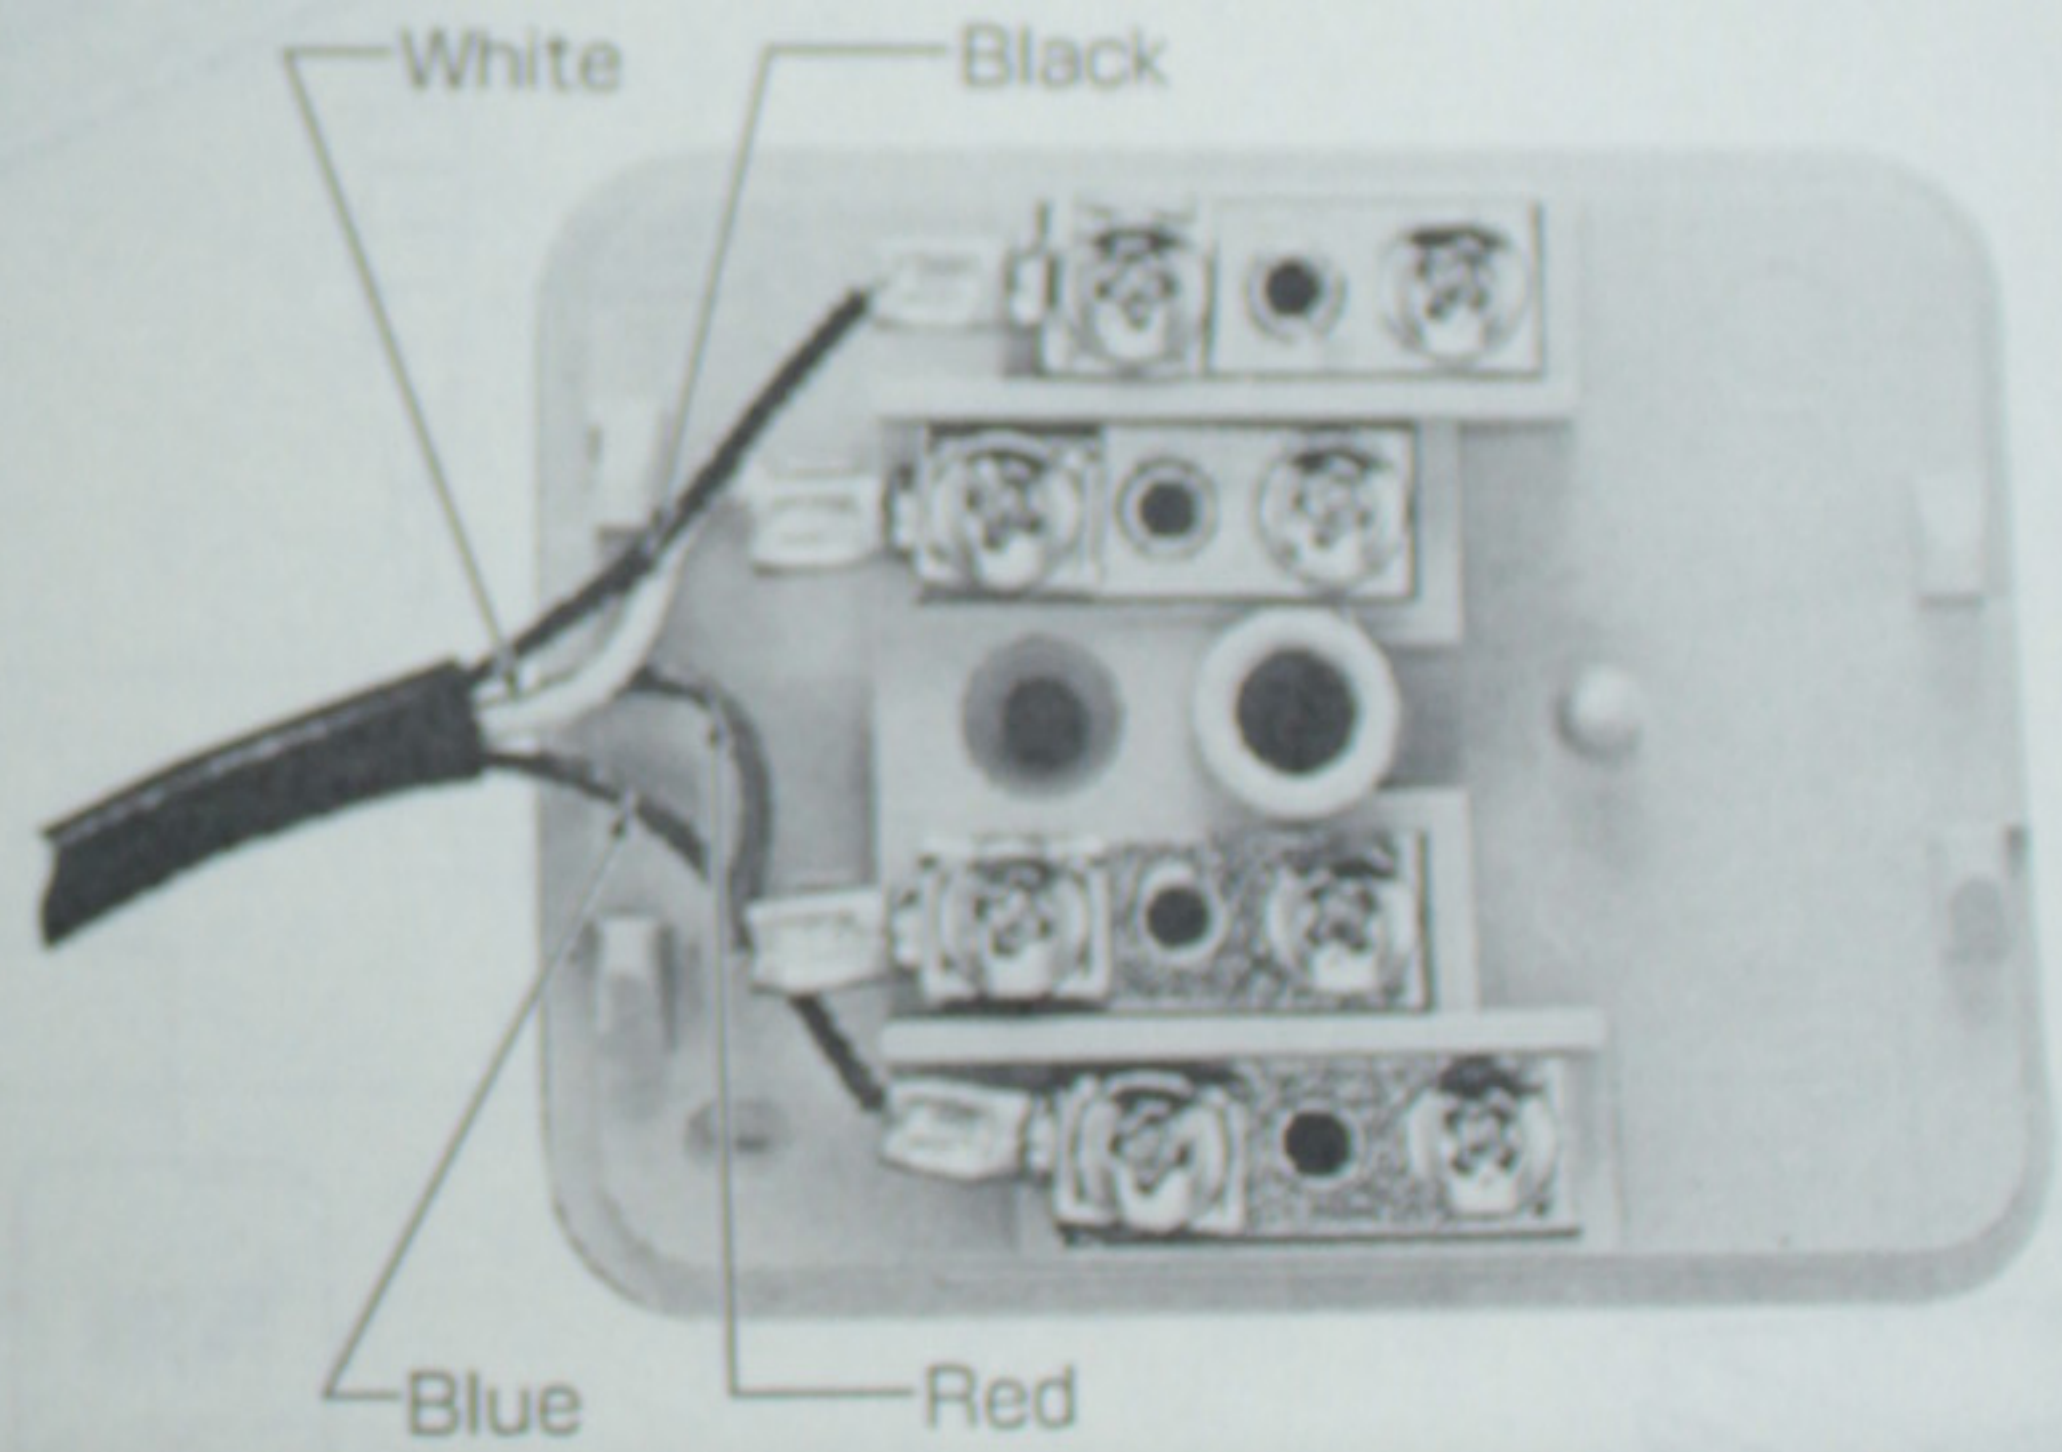

Terminal box (Inside)

## Standard specification

Description	Specification
Plug	4 pins
Signal wire	Oil-resistant vinyl round-core wire 0.2mm <sup>2</sup> x 4C
Terminal box (To replay signals)	For indoor communication wire, 4 terminals

# 13. SIGNAL WIRE UNIT (OPTION)

TBX-SS-B


The signal wire unit is to connect the meter with a remote display, a counter, etc., which is consisted of 2m signal wire with the plug and the terminal box to replay signals.




Signal wire (2m) with plug

## Connection method to utilize output signal

Kind of flow pulse	Unit pulse		High density pulse	
Color of signal wires	Red	Blue	White	Black
Polarity of terminals	+	-	+	-

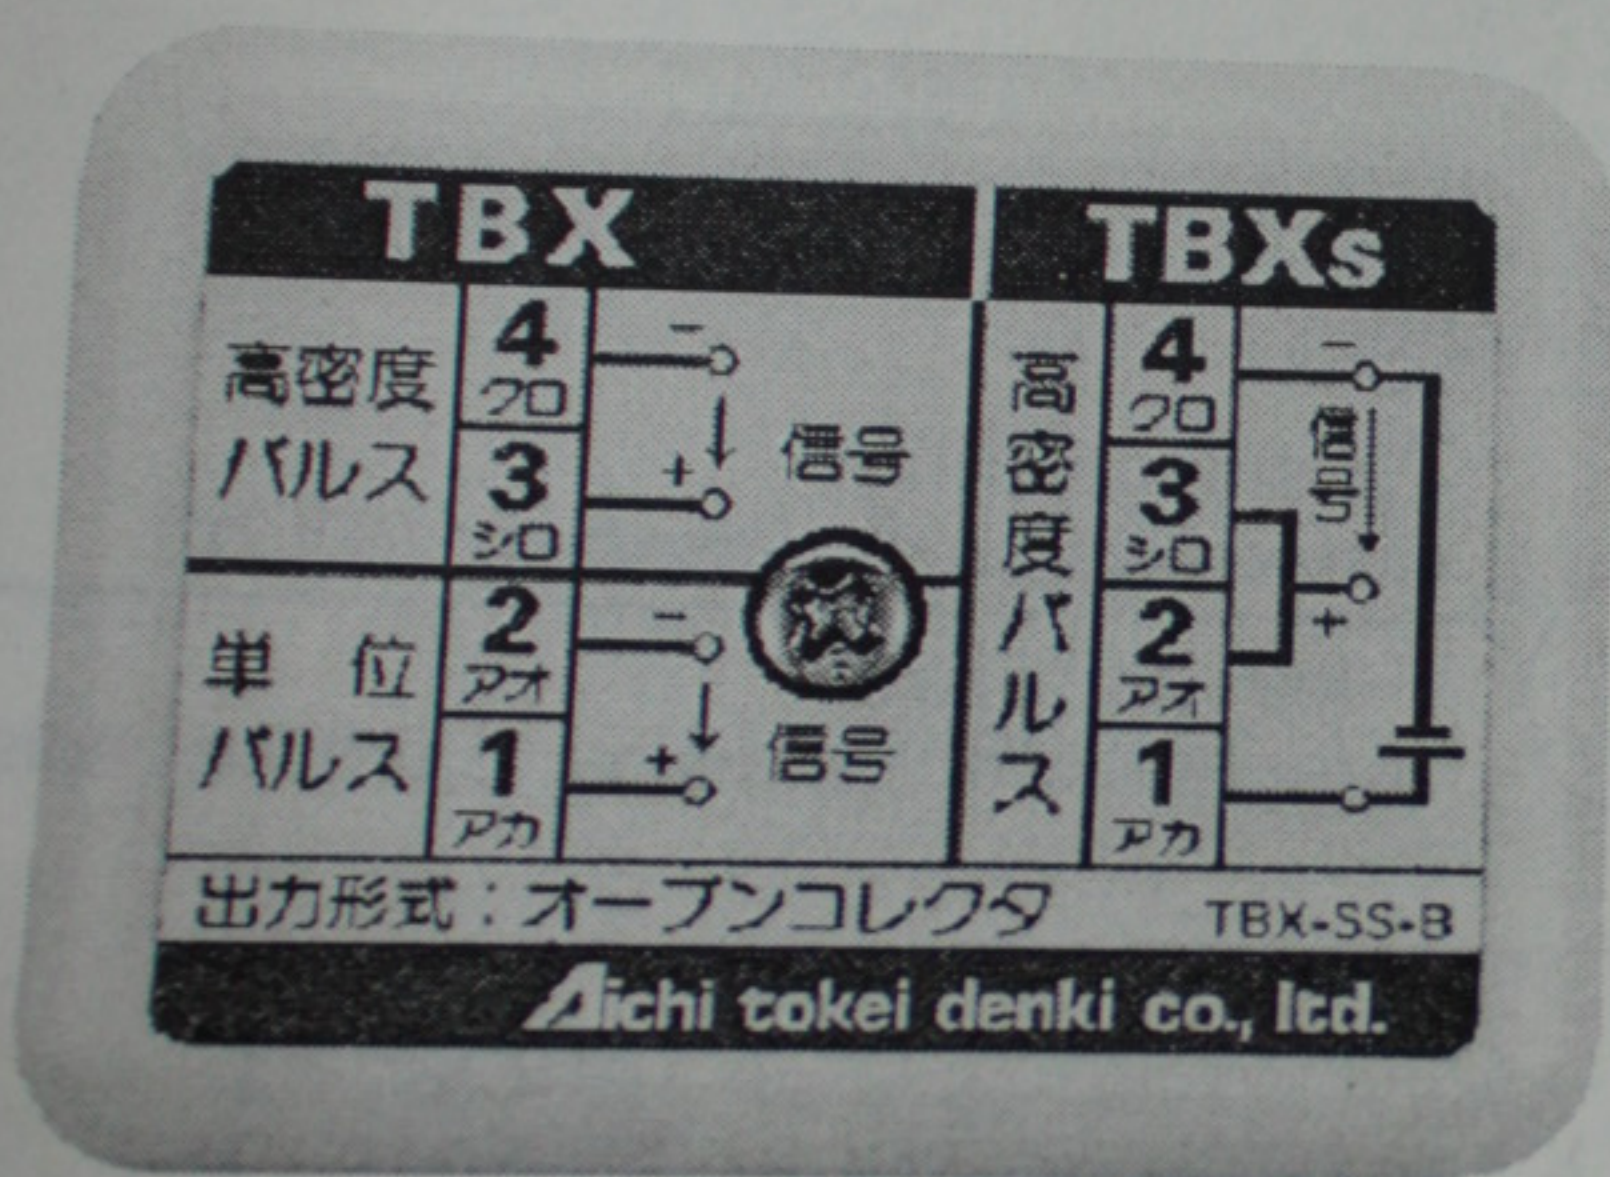

Terminal box (Outside)

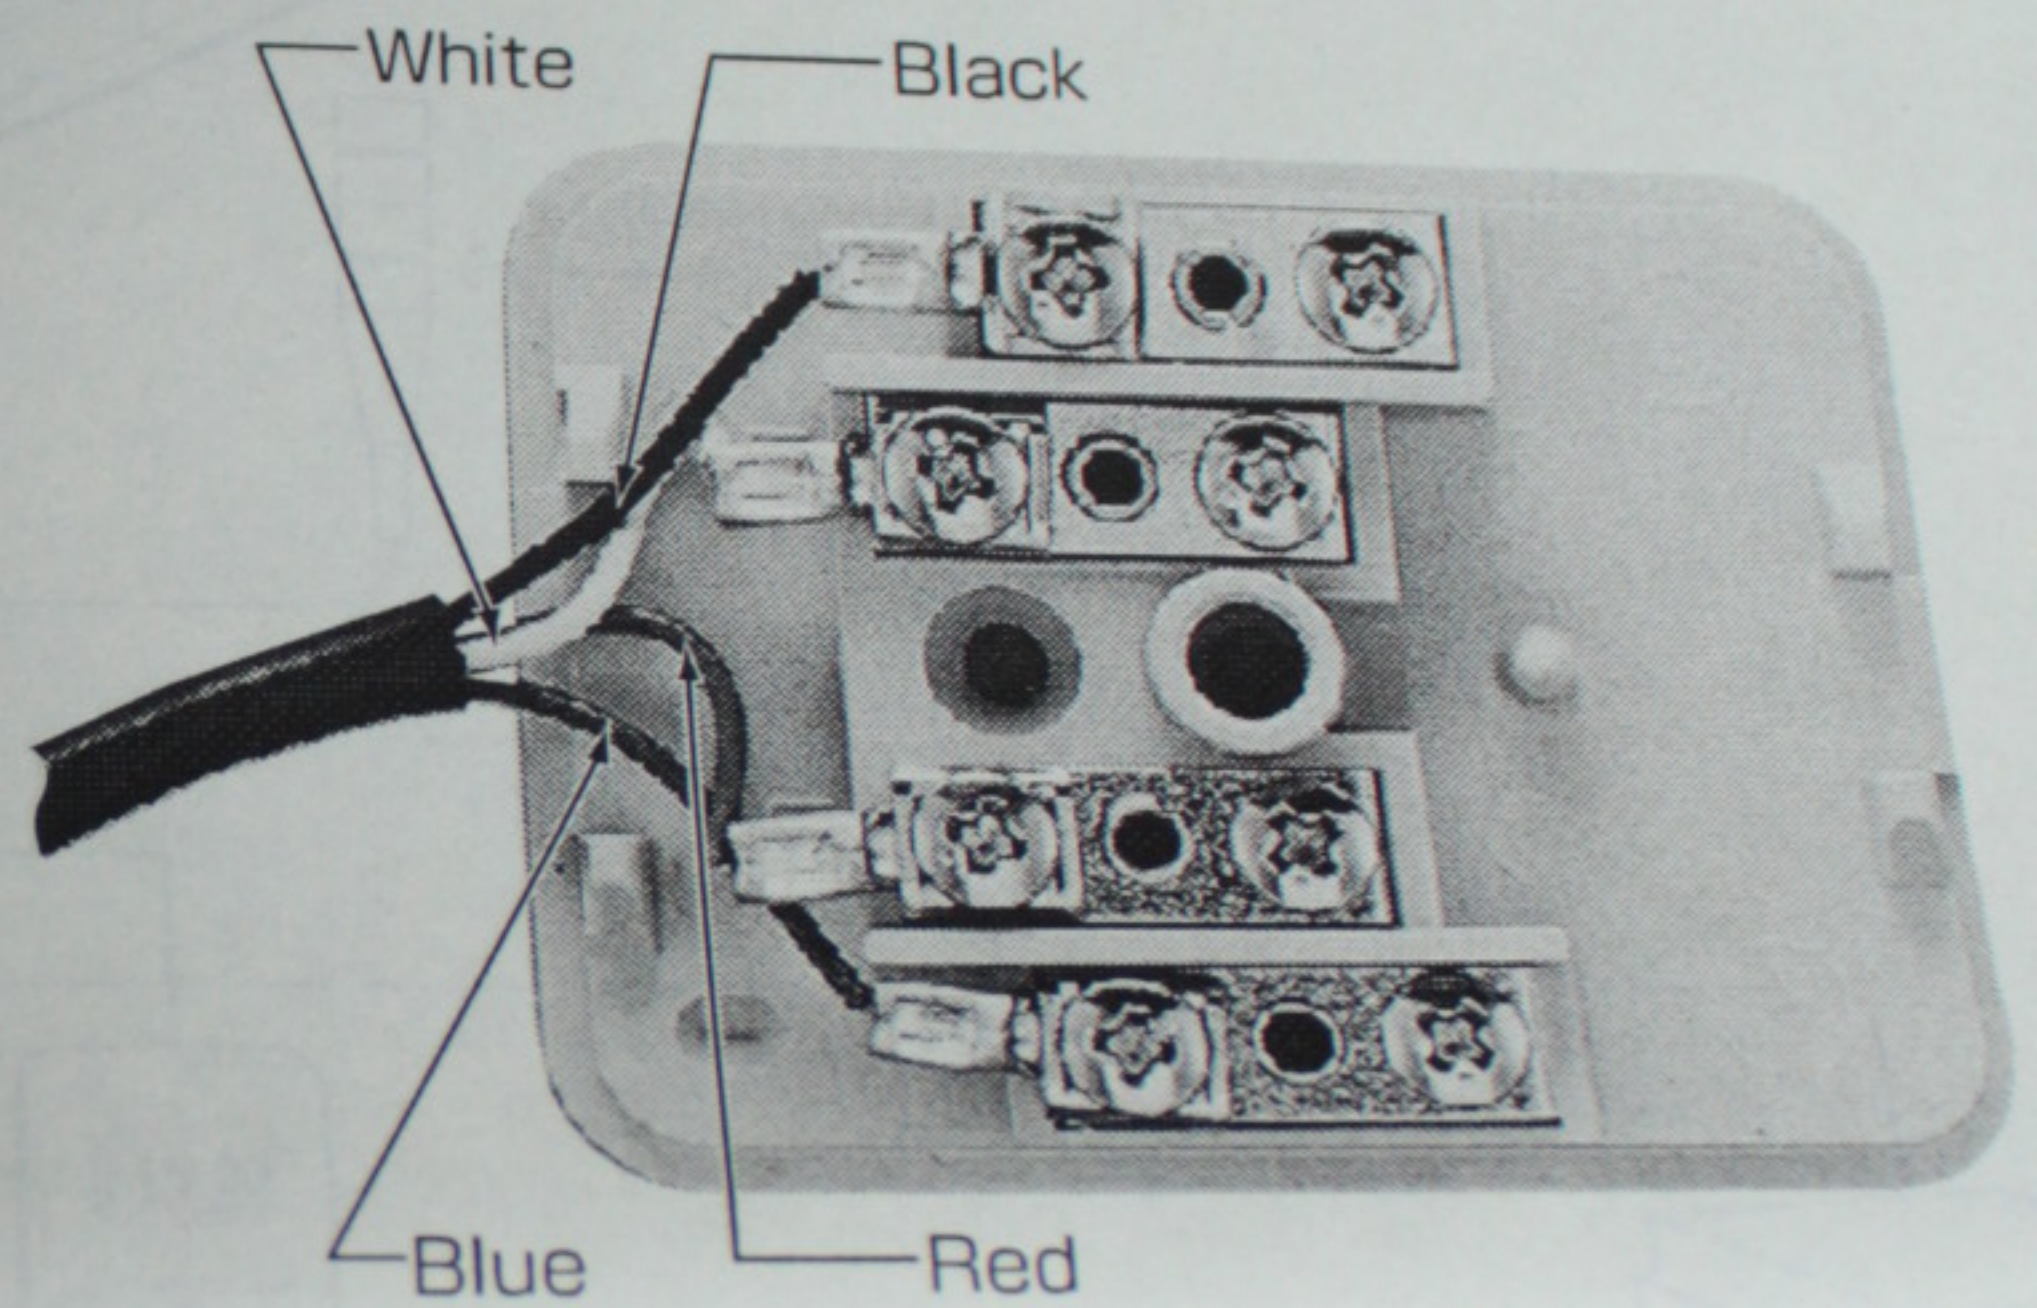

Terminal box (Inside)

## Standard specification


Description	Specification
Plug	4 pins
Signal wire	Oil-resistant vinyl round-core wire $0.2\text{mm}^2 \times 4C$
Terminal box (To replay signals)	For indoor communication wire, 4 terminals

# 14. REMOTE DISPLAY / COUNTER (OPTION)

## 1) Kind of Remote displays / counters

Model	Functions, etc.	Power supply
ZC09-96	Instantaneous flow indication, integrating flow indication, and pulse signal output	Built-in battery
ZX-562	Instantaneous flow indication, integrating flow indication, analog signal output, and alarm signal output	AC85V ~ AC264V
PM10Z	Integrating printer (with display)	AC100V
RE101	Recorder	Selectable from AC100V type, AC200V type, and DC24V type

## 2) System example

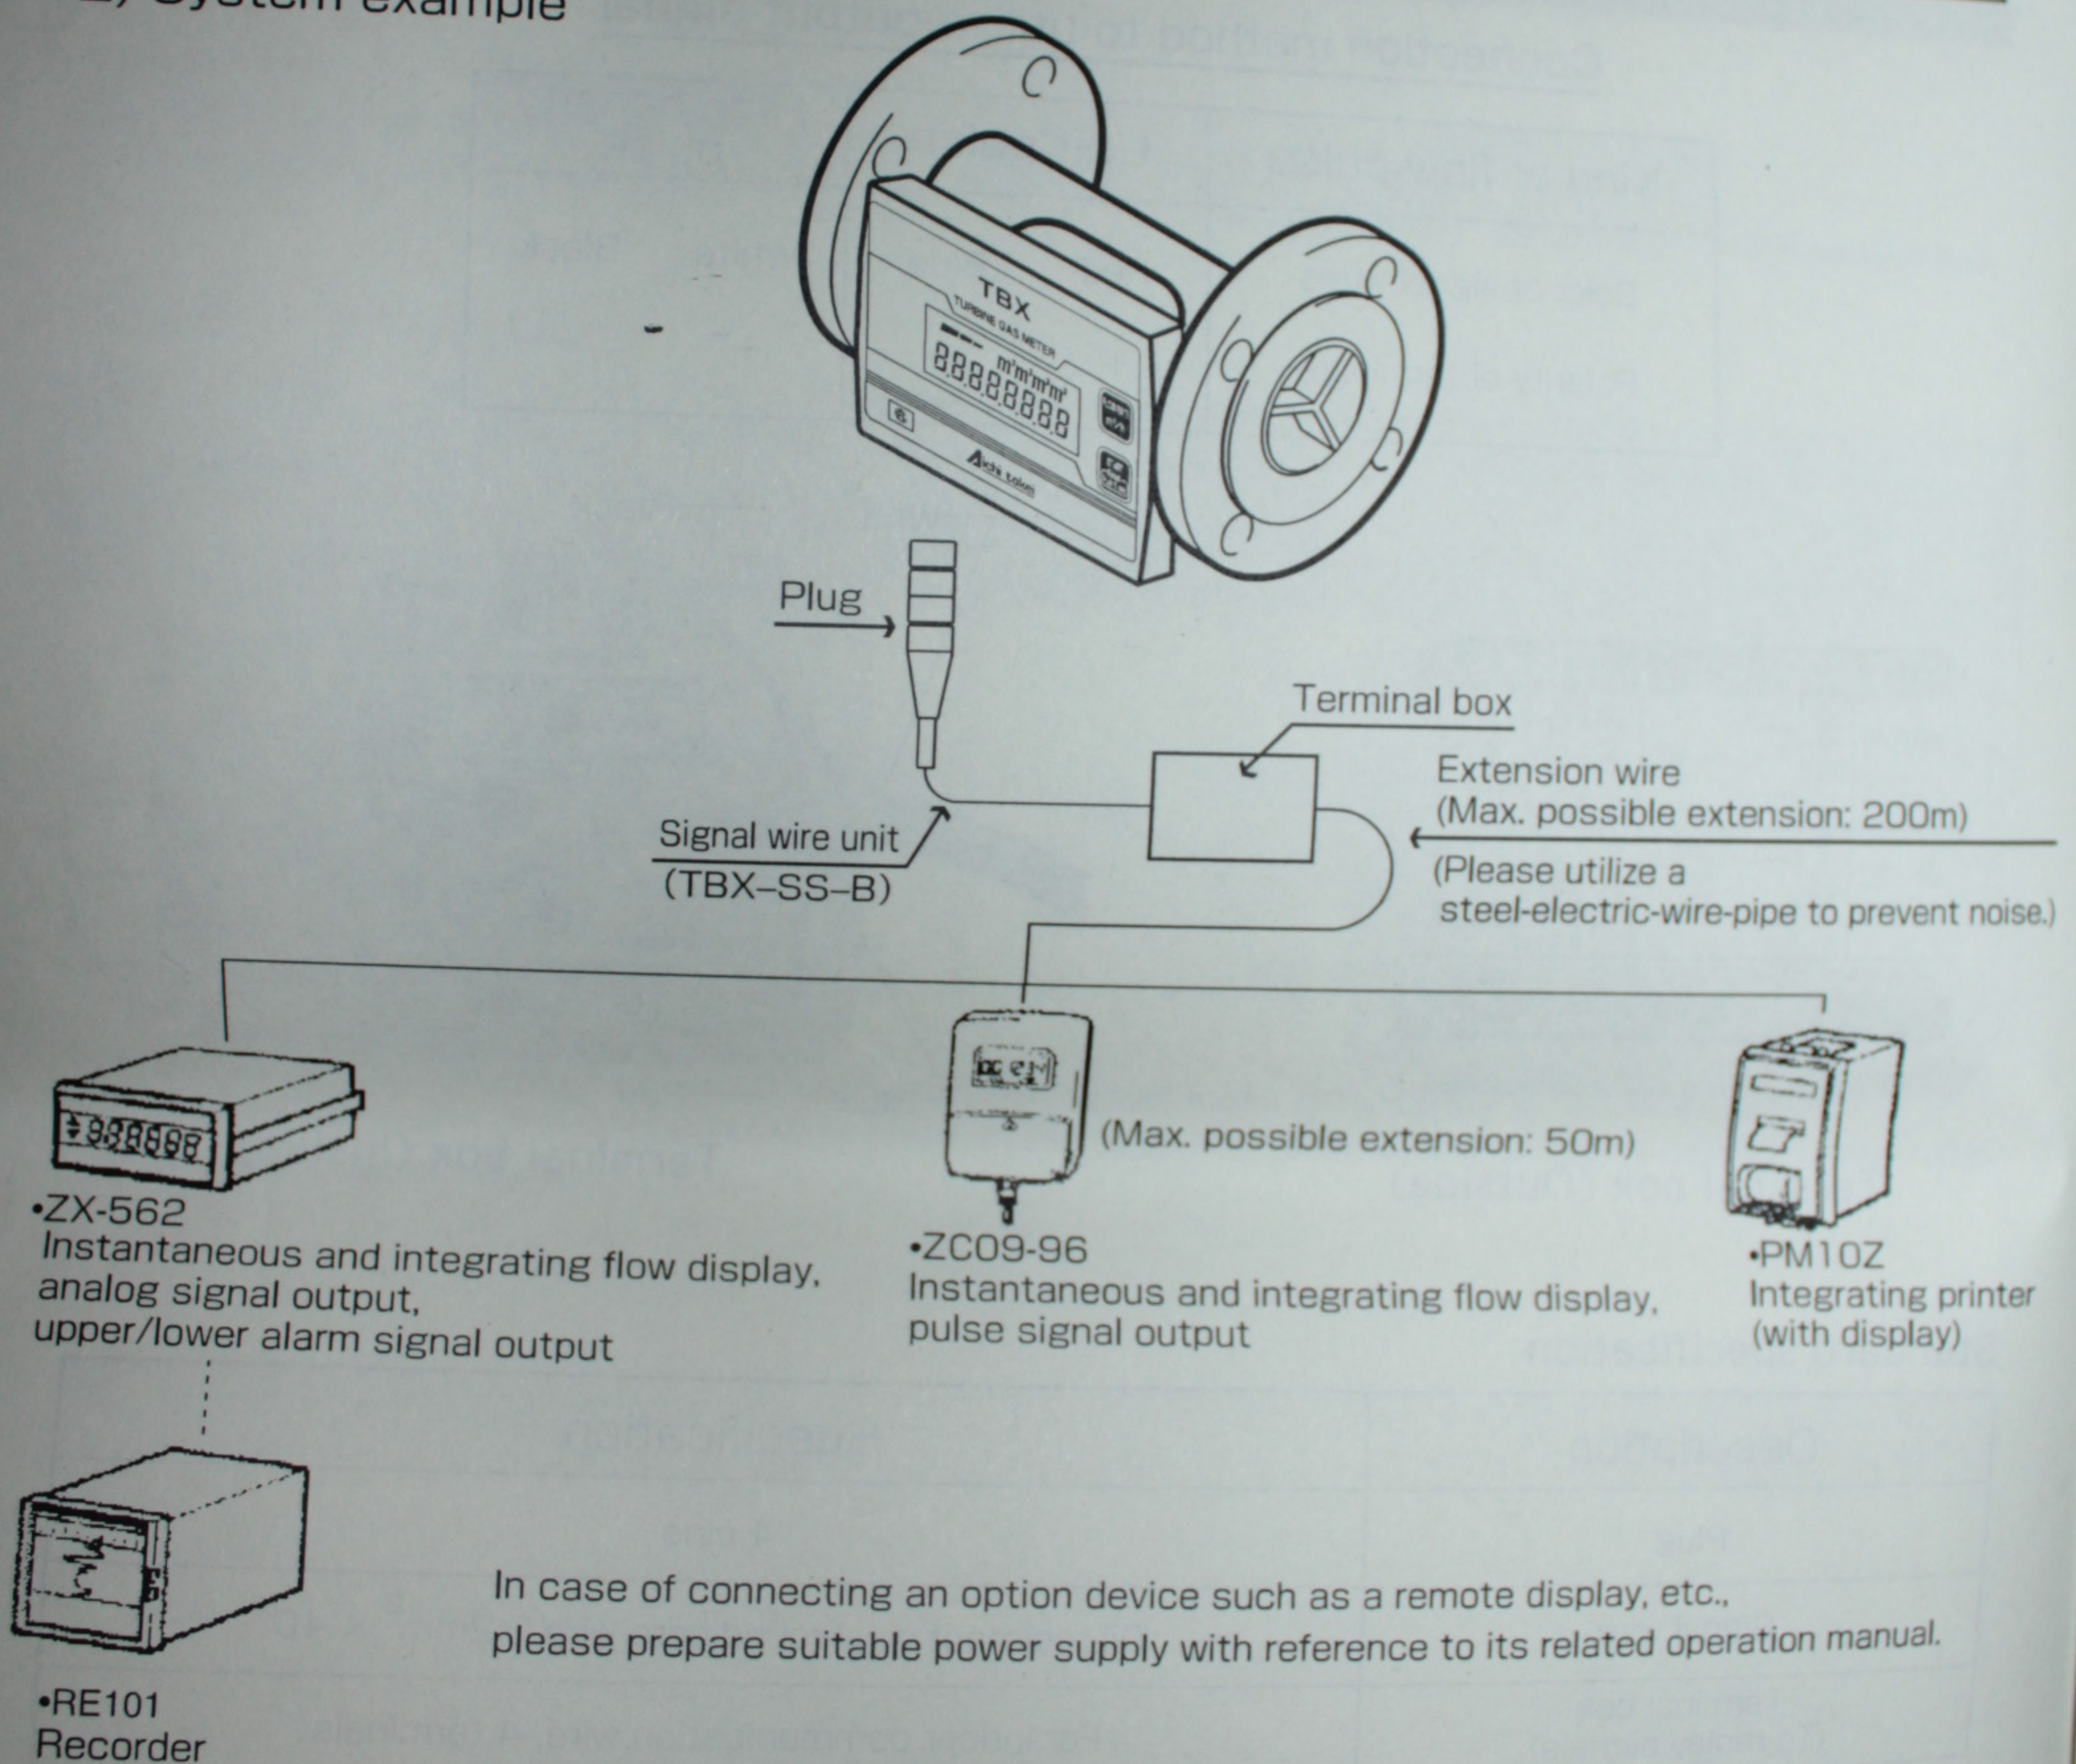

## 15. WARRANTY

Aichi warrants its products only defects in materials and workmanship and this warranty extends for a period of one year from the date of Aichi's shipment.

This warranty does not apply to any goods which have been ( I ) repaired, altered, or improperly installed; ( II ) subjected to improper use or storage; ( III ) used or incorporated, with other materials or equipment, or after anyone using the goods has or reasonably should have knowledge of any defect or nonconformance of the goods; or ( IV ) manufactured, fabricated or assembled by anyone other than Aichi; ( V ) damaged arising through an act of god.